

# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR®

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2




# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

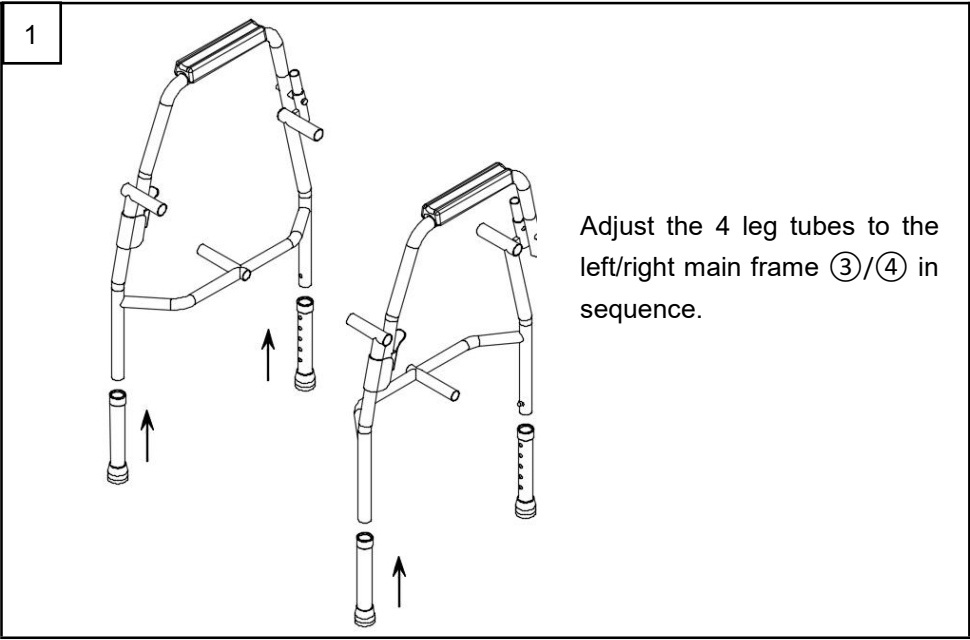

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

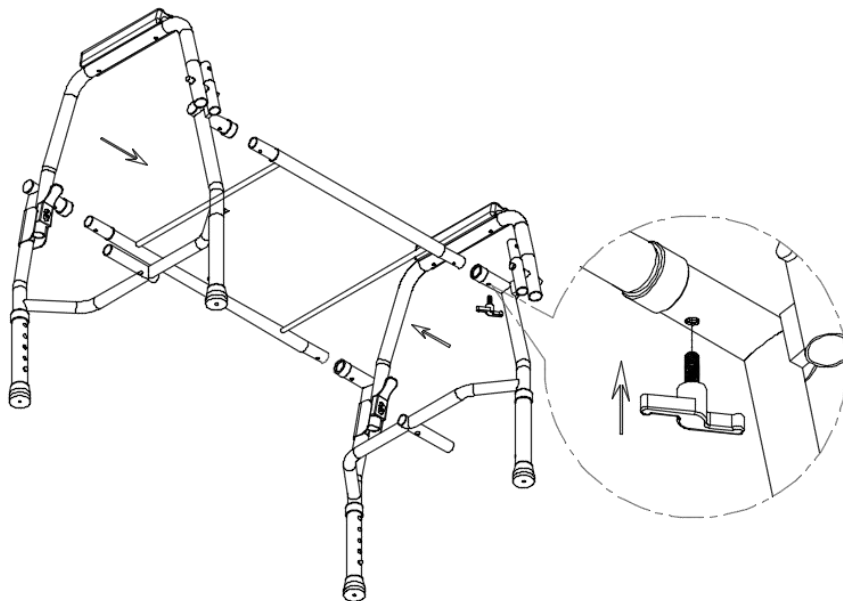


3

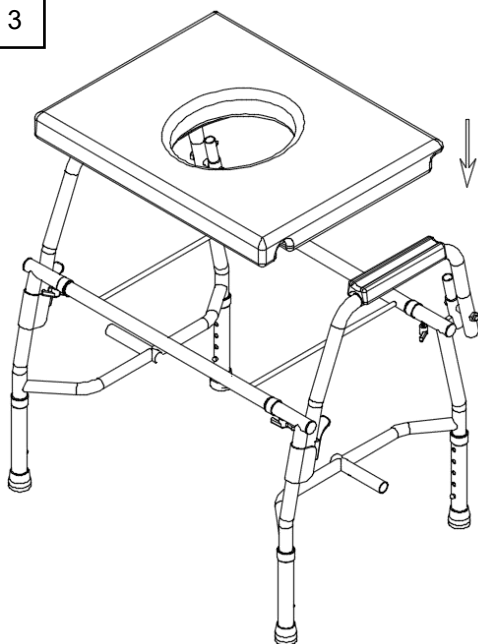


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

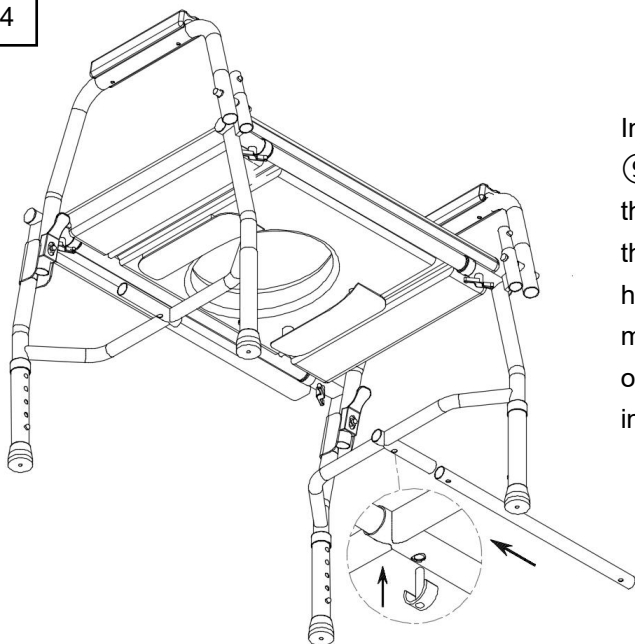


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

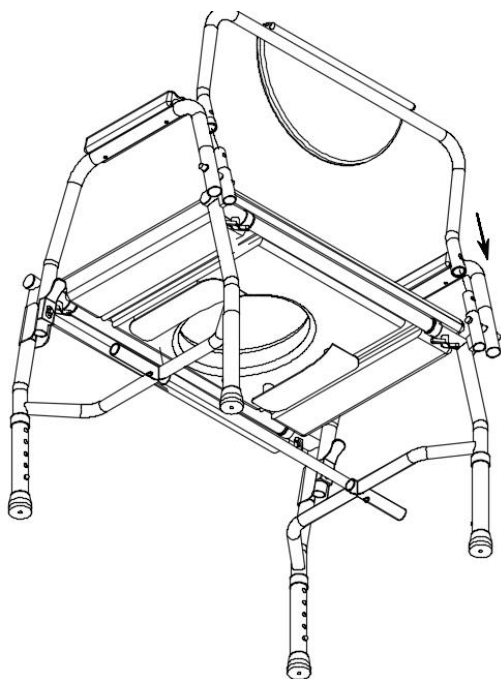

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

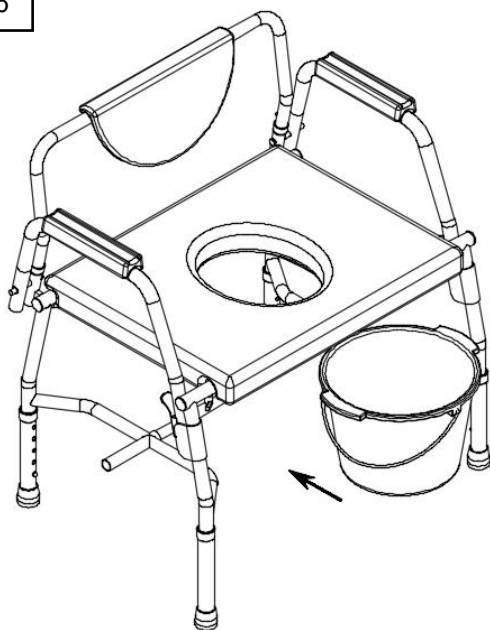

Place the pail⑤ through the front of the seat frame.


7

(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

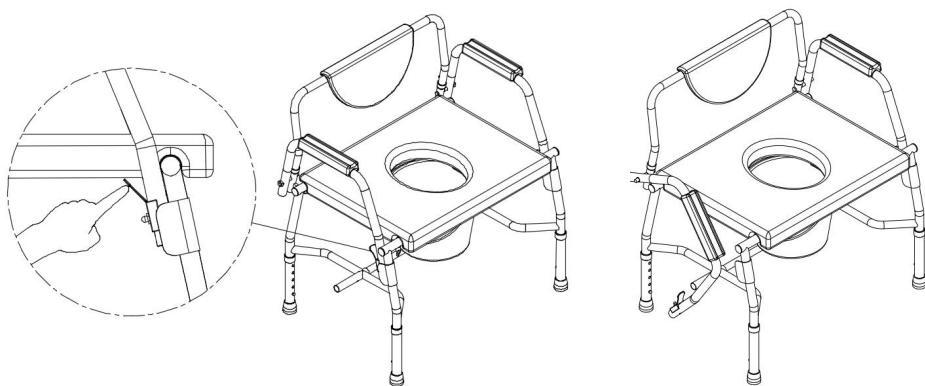


8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

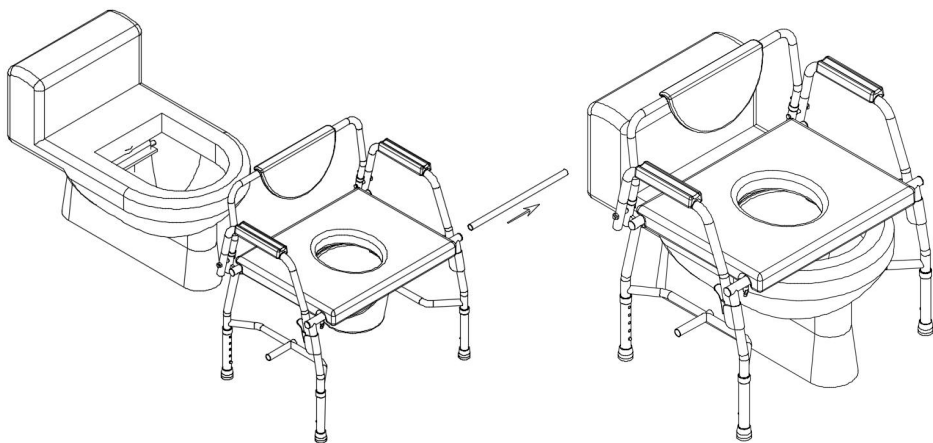

9

Toilet height adjustment, press the marble to pull the legs out and so on.

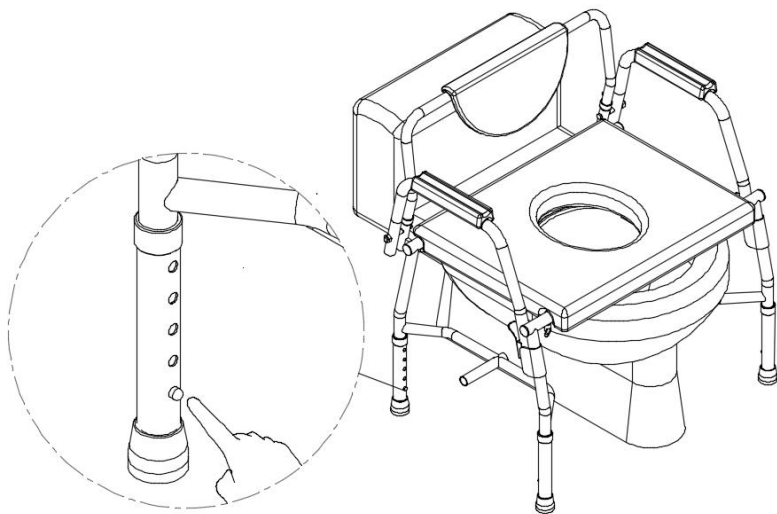

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR<sup>®</sup>

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.


NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2

# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

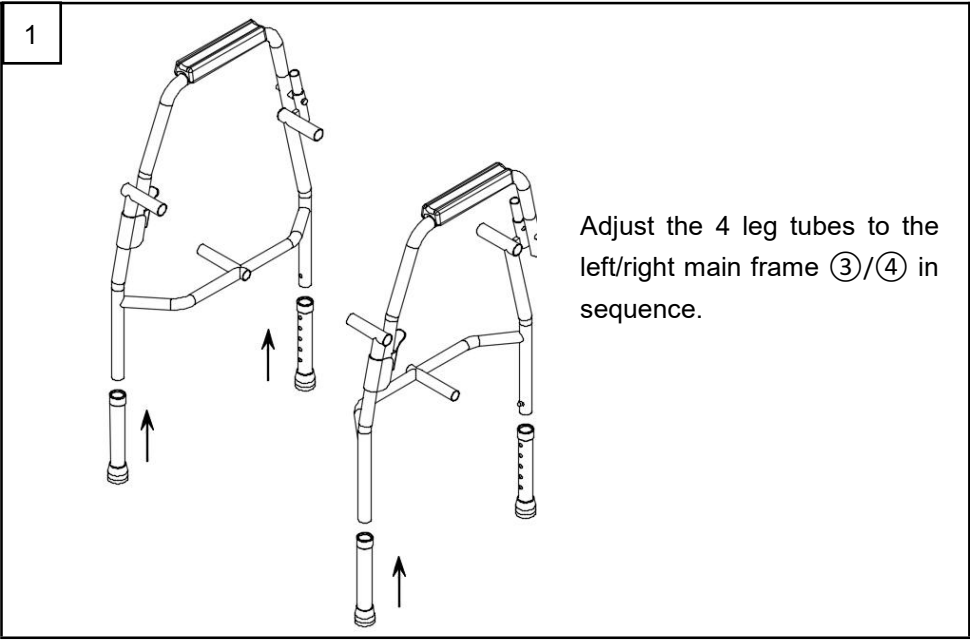

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

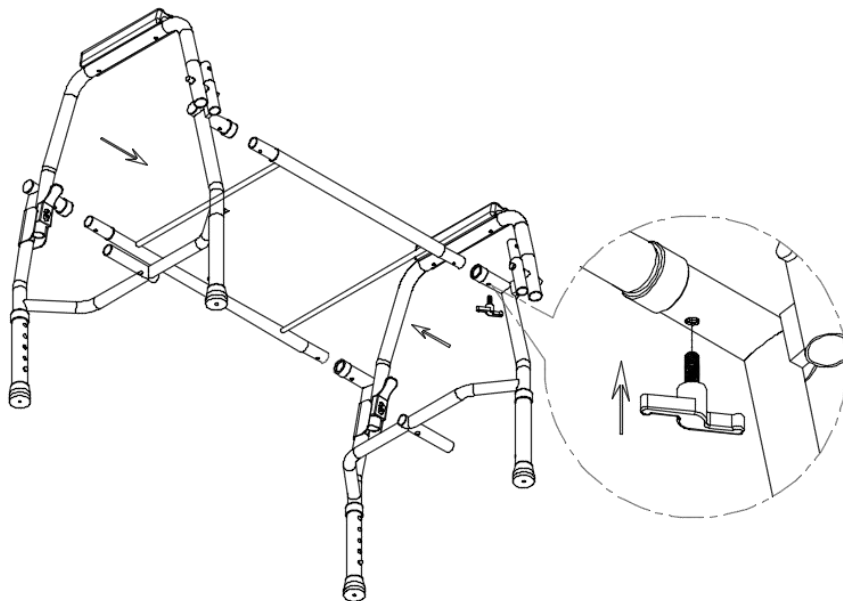


3

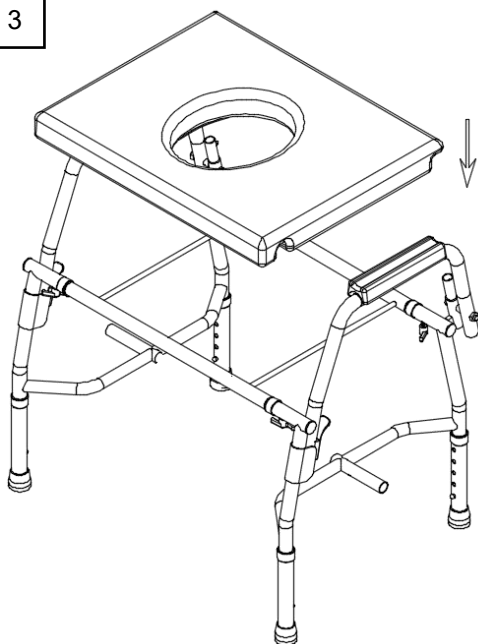


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

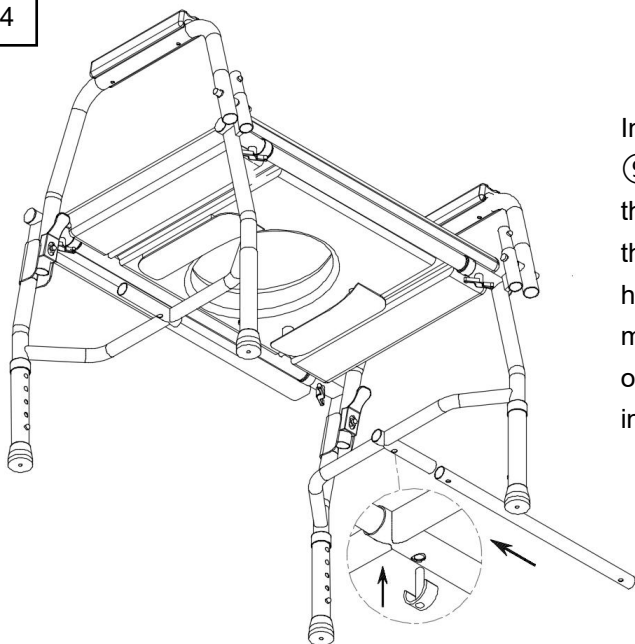


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

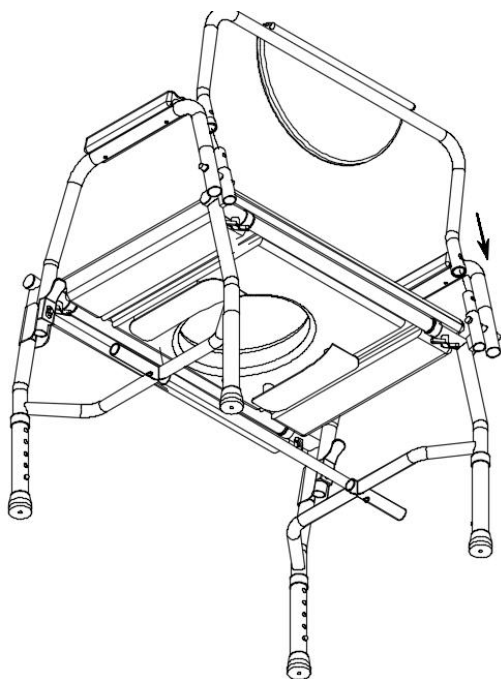

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

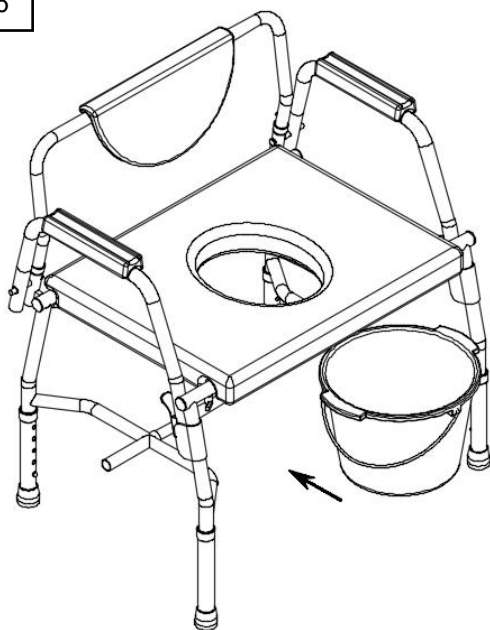

Place the pail⑤ through the front of the seat frame.

7


(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

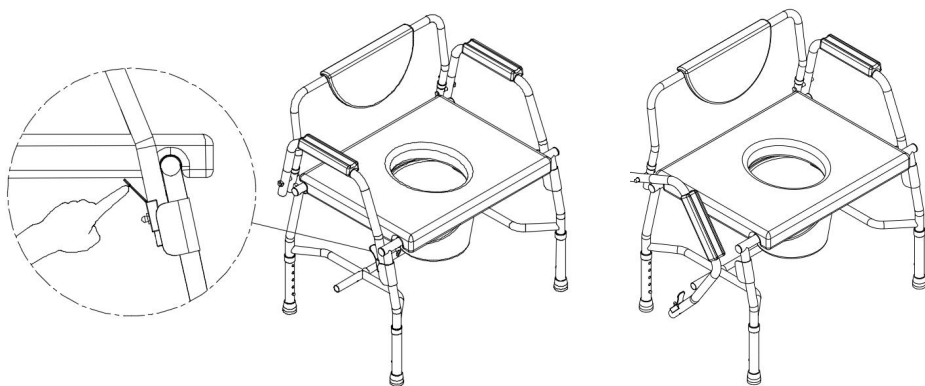




8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

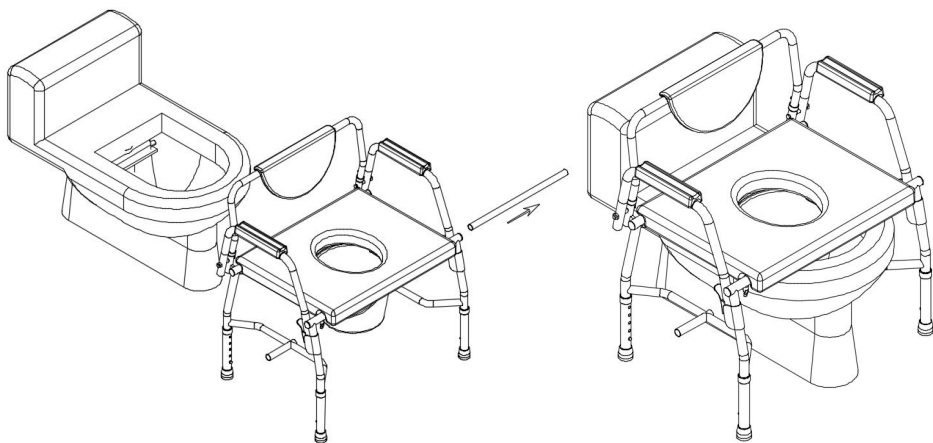

9

Toilet height adjustment, press the marble to pull the legs out and so on.

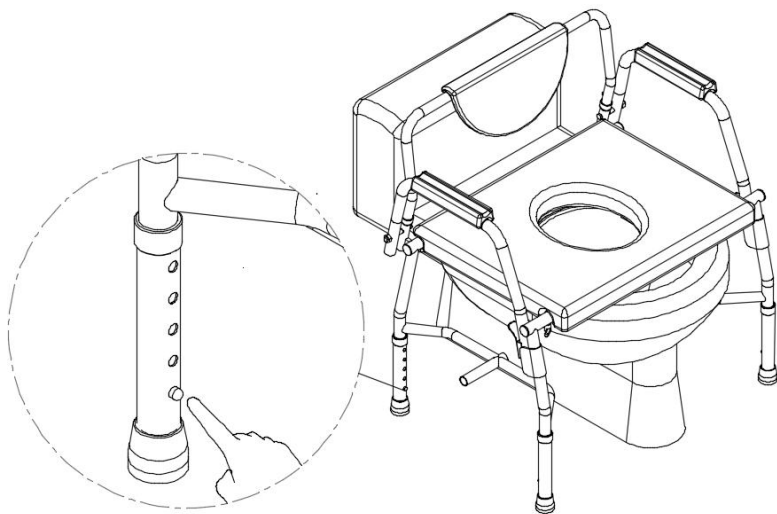

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**

# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR®

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2




# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

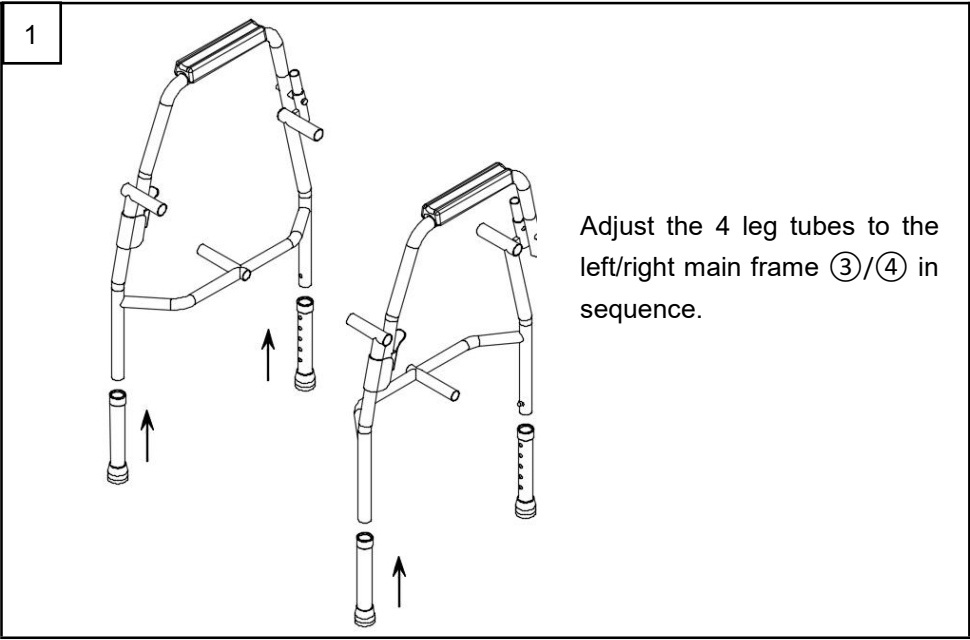

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

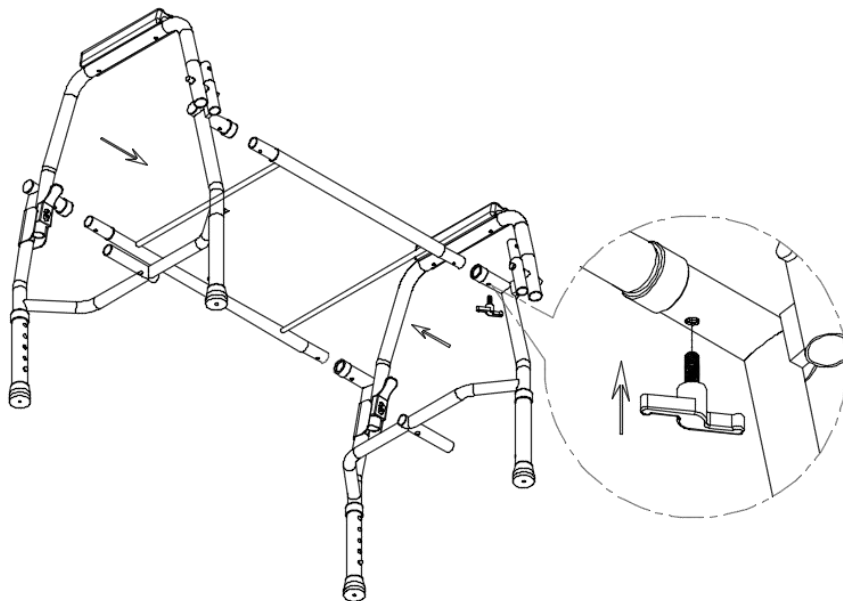


3

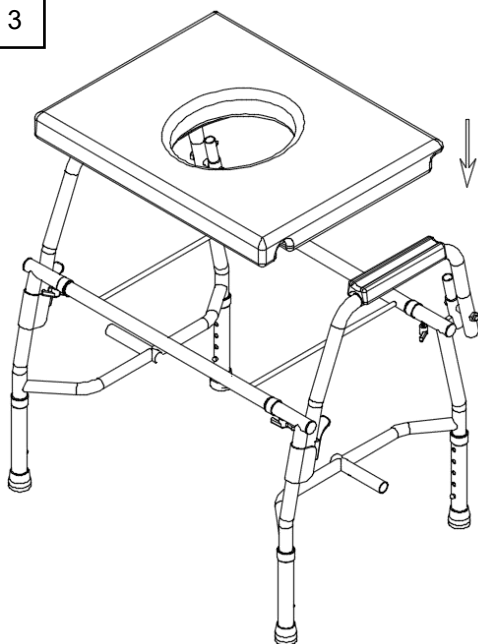


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

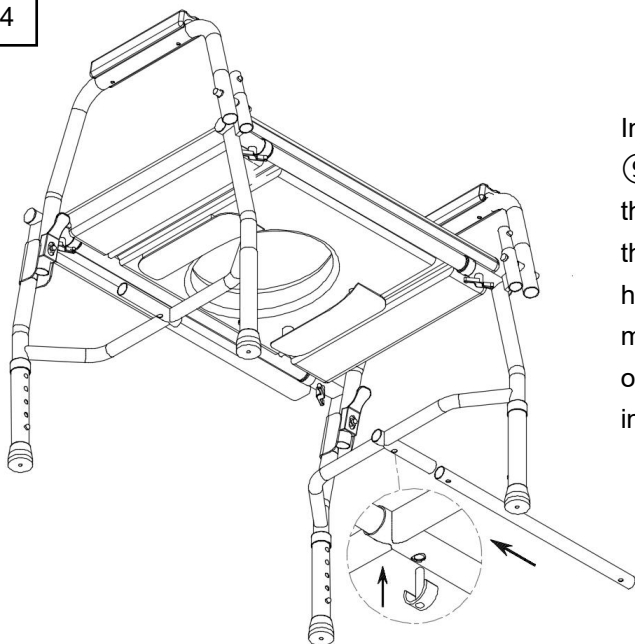


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

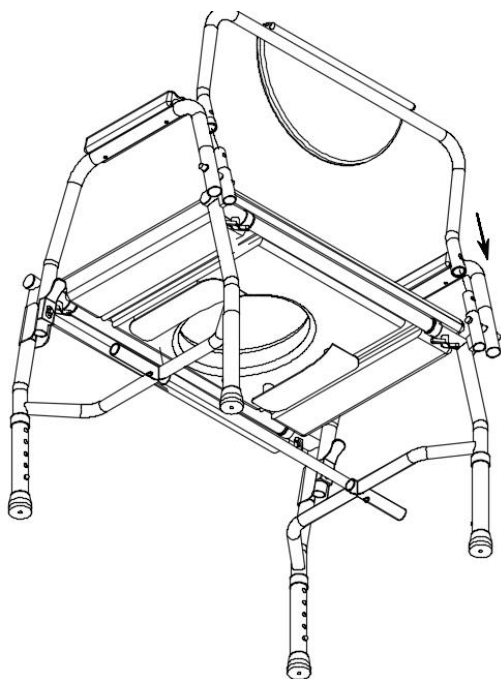

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

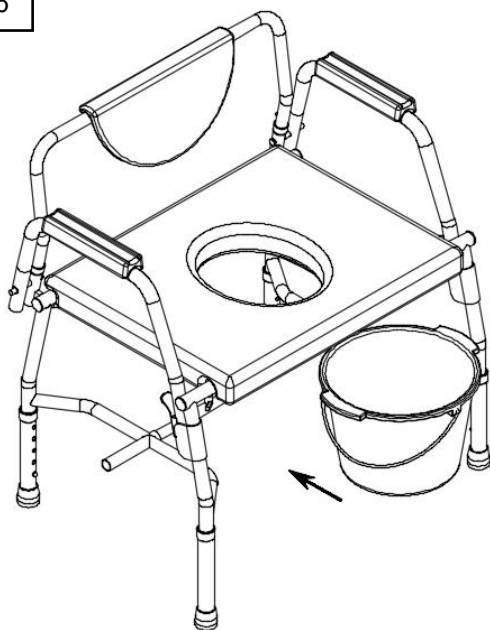

Place the pail⑤ through the front of the seat frame.


7

(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

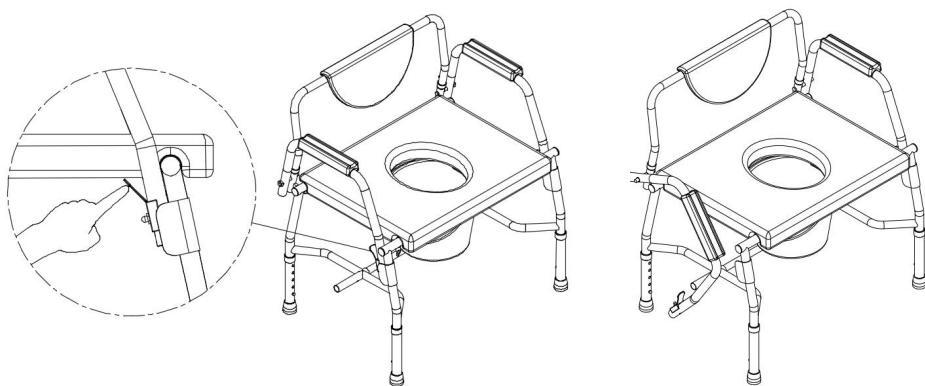


8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

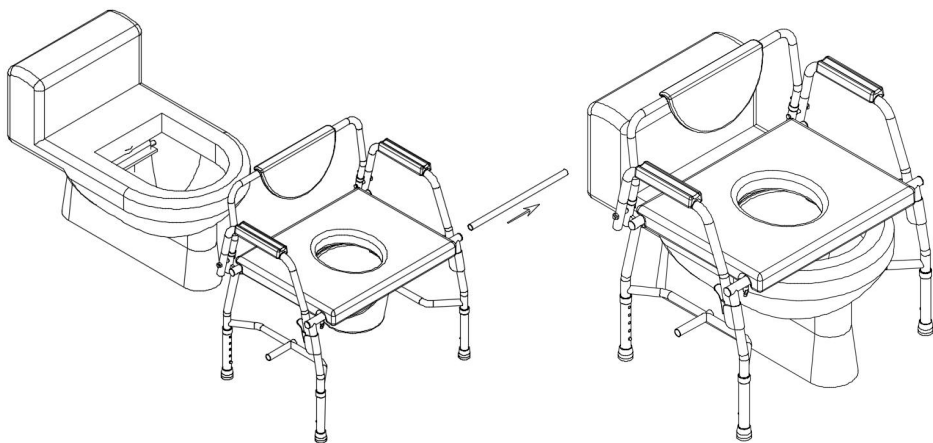

9

Toilet height adjustment, press the marble to pull the legs out and so on.

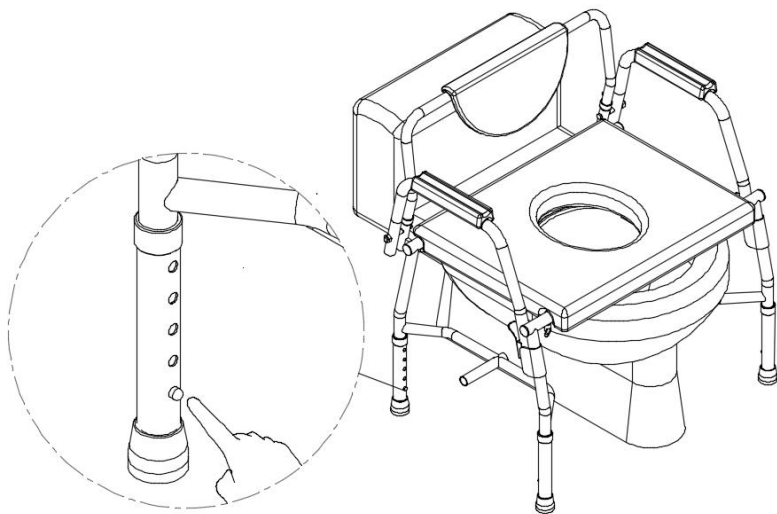

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR<sup>®</sup>

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.


NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2

# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

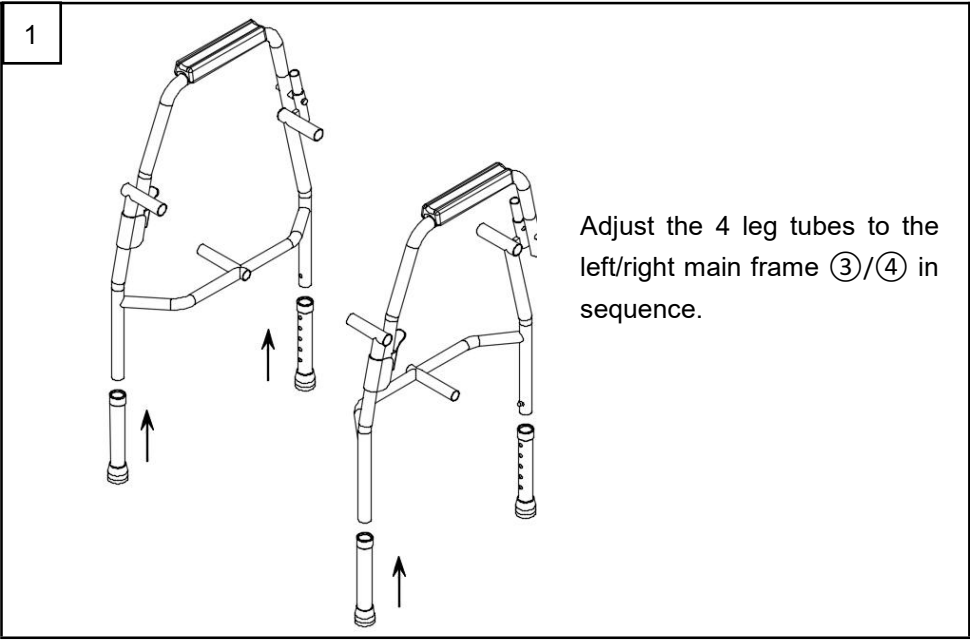

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

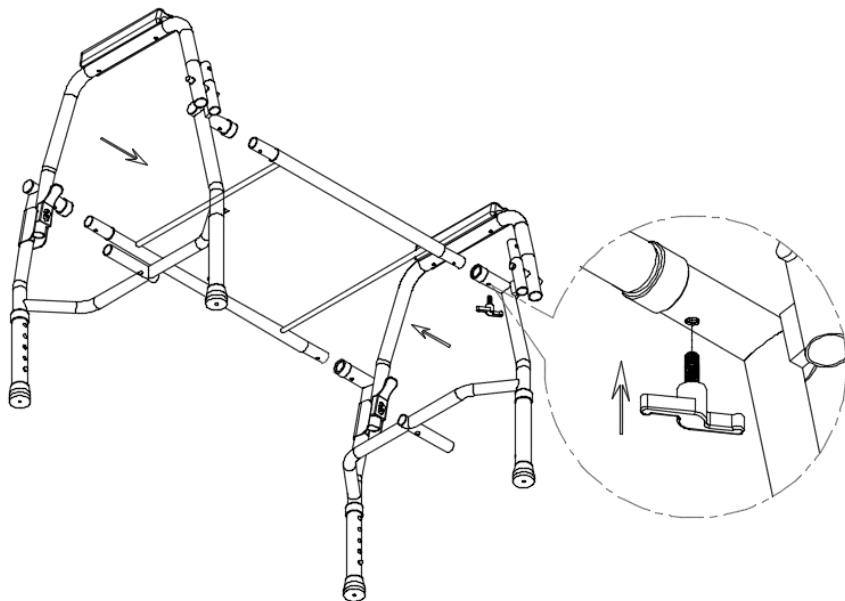


3

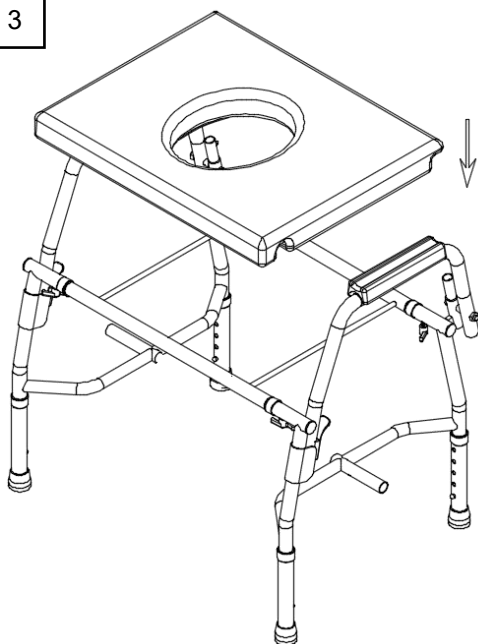


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

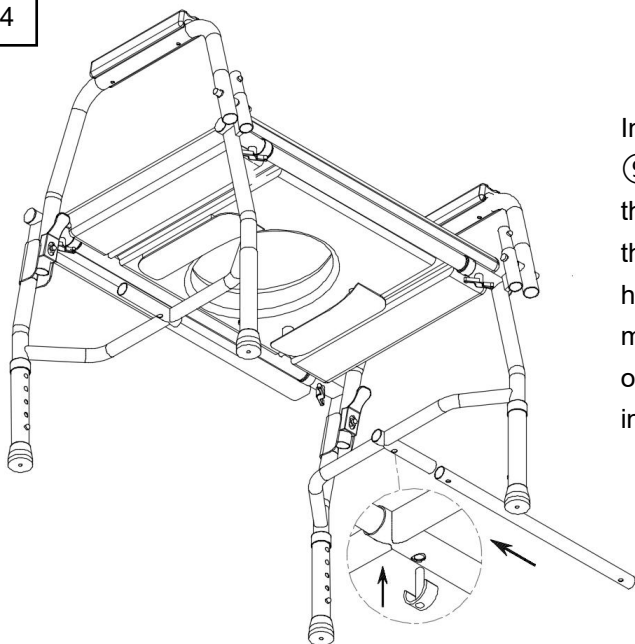


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

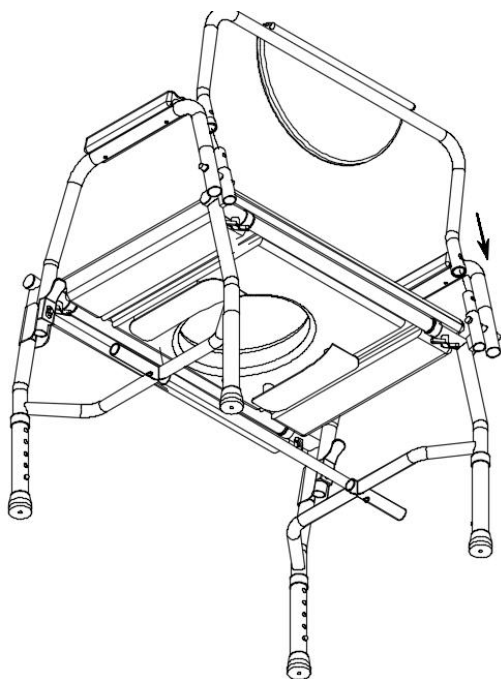

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

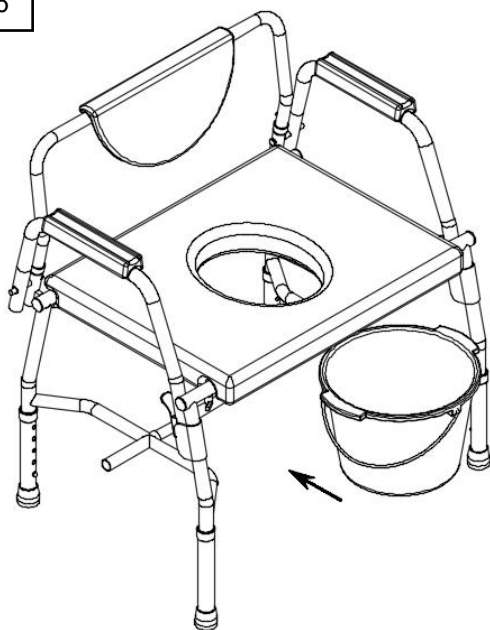

Place the pail⑤ through the front of the seat frame.

7


(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

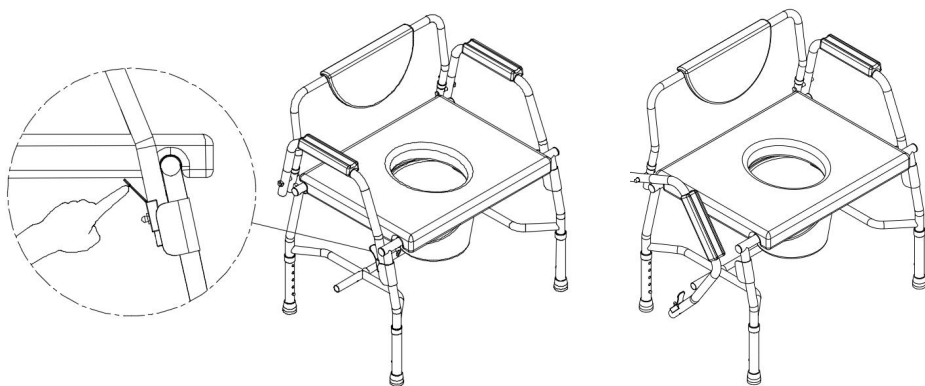




8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

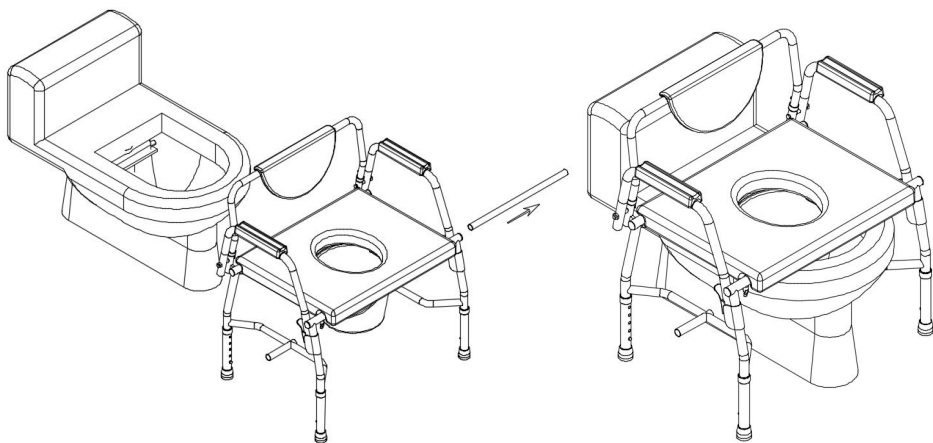

9

Toilet height adjustment, press the marble to pull the legs out and so on.

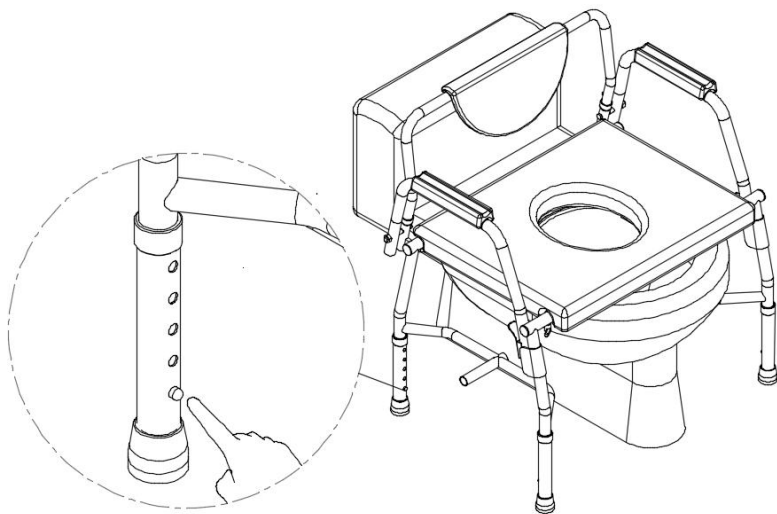

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**

# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR®

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2




# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

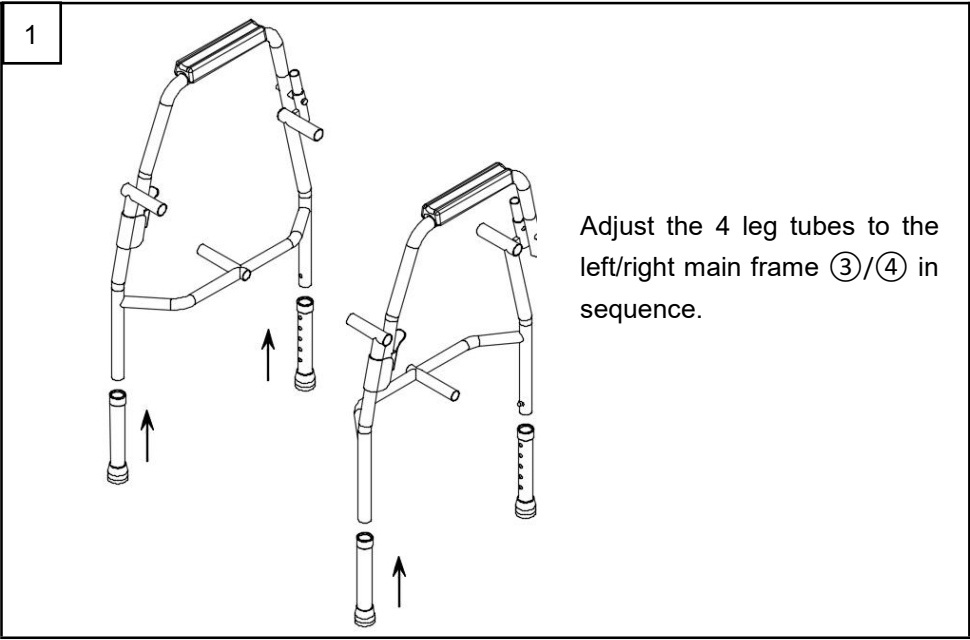

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

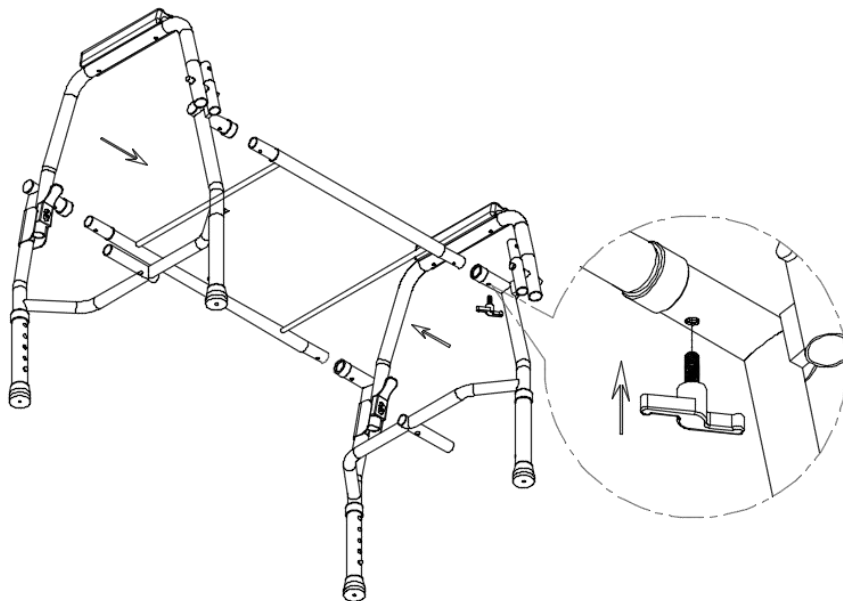


3

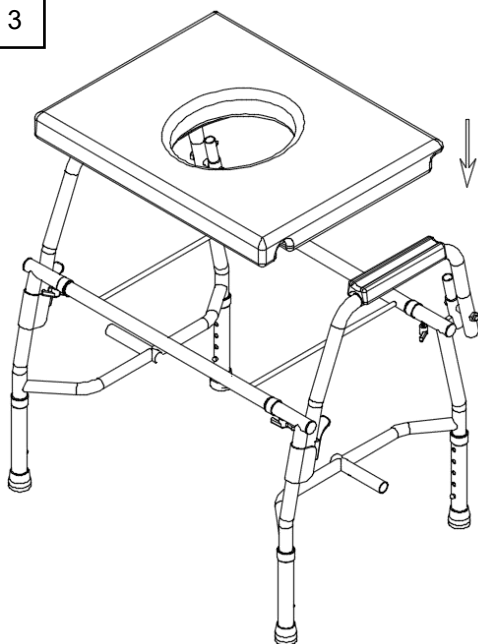


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

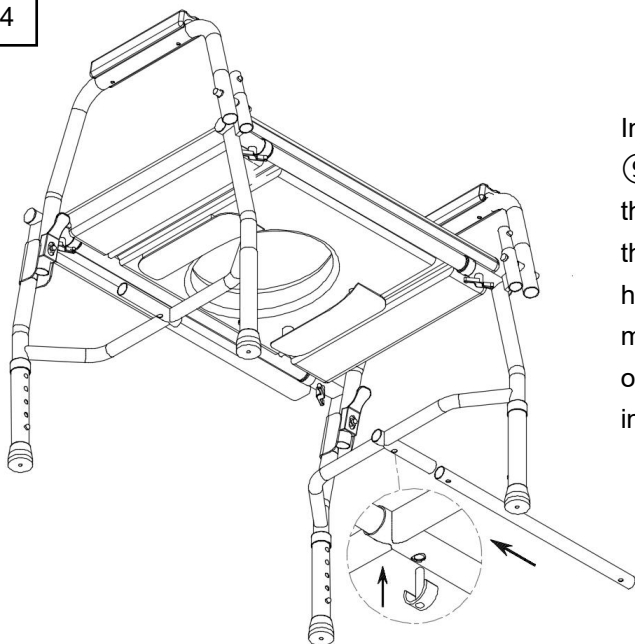


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

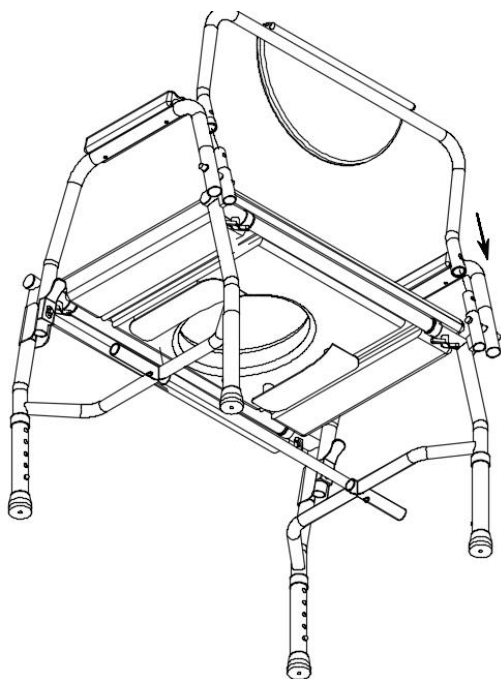

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

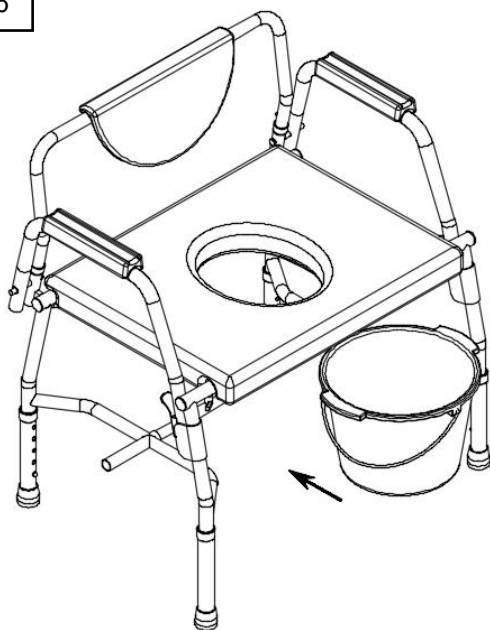

Place the pail⑤ through the front of the seat frame.


7

(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

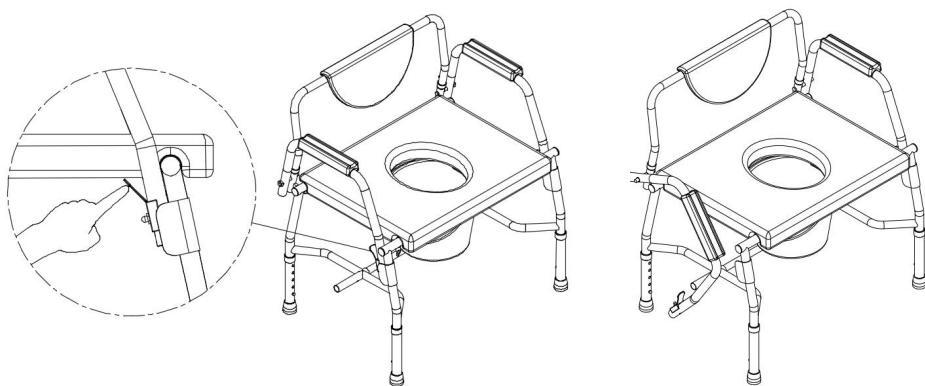


8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

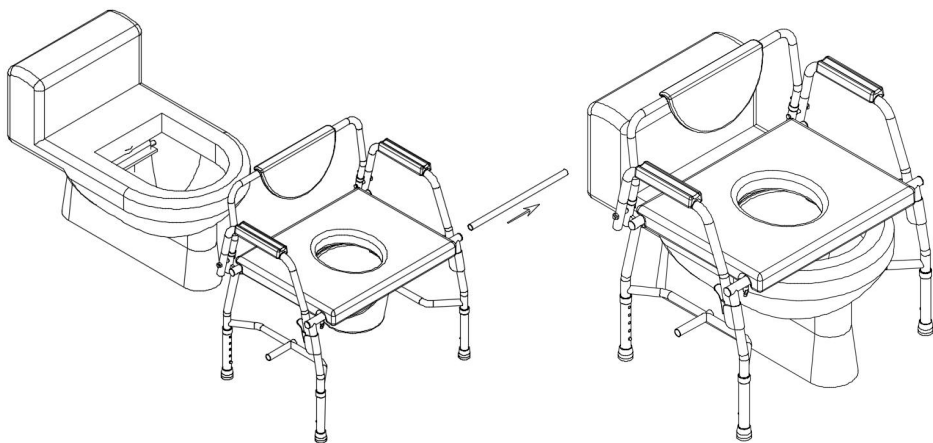

9

Toilet height adjustment, press the marble to pull the legs out and so on.

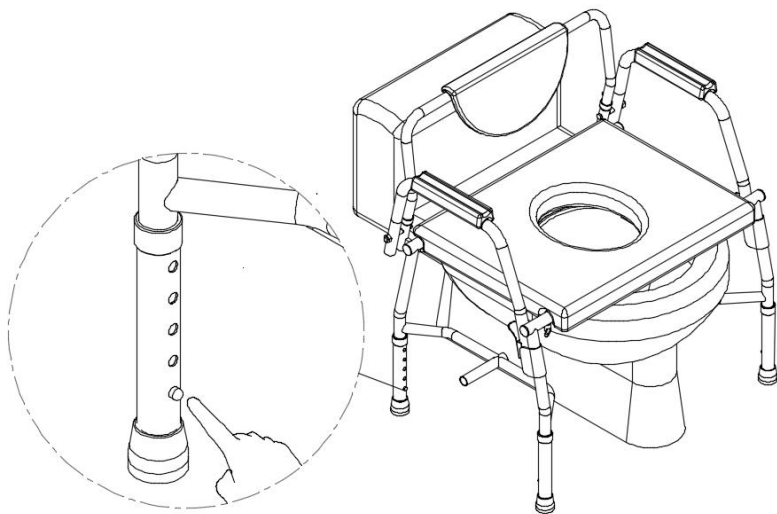

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR<sup>®</sup>

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.


NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2

# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

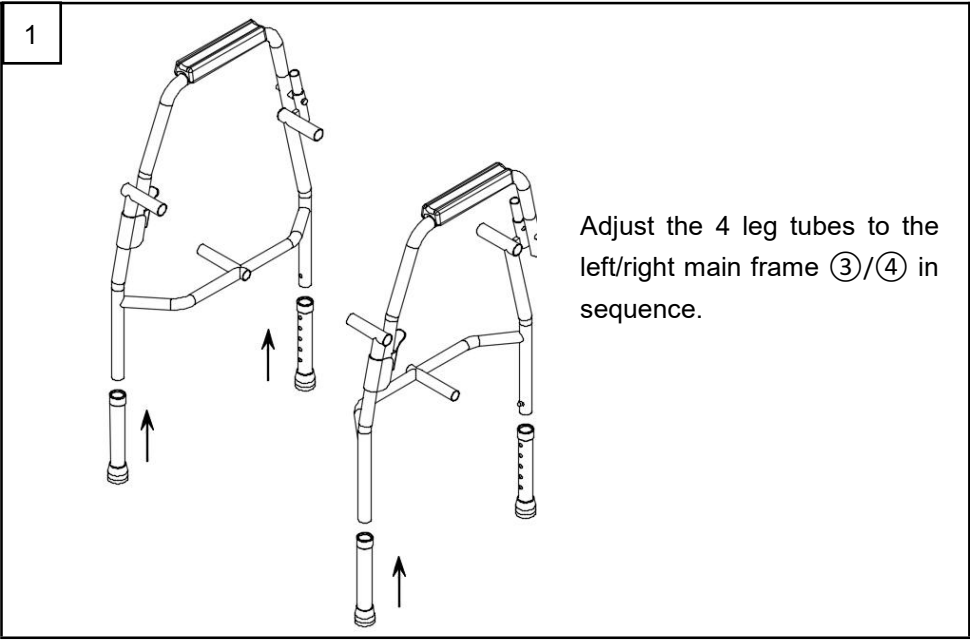

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

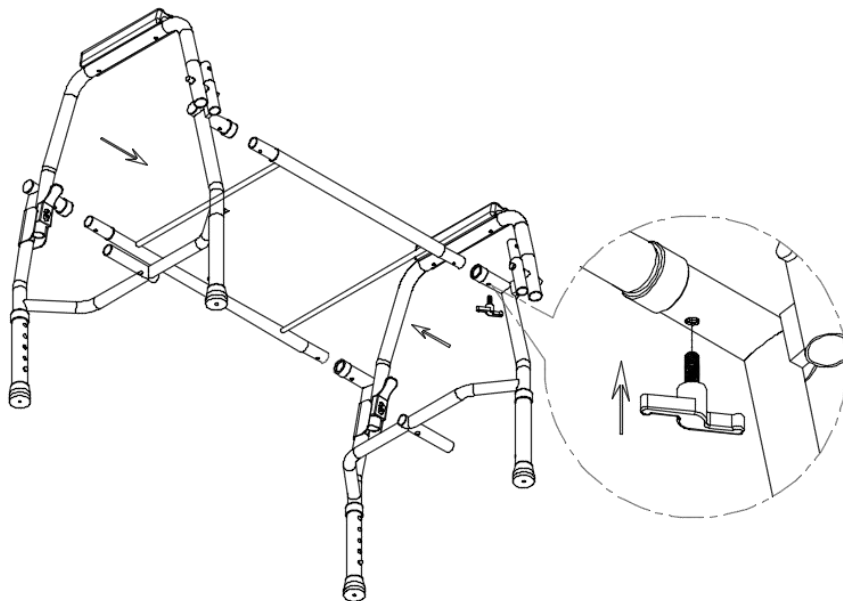


3

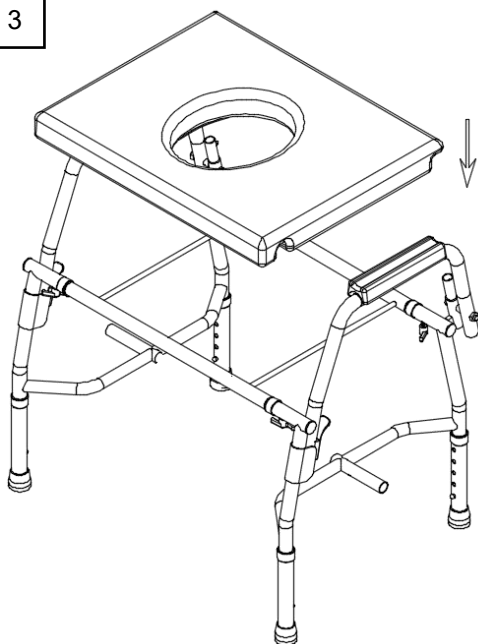


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

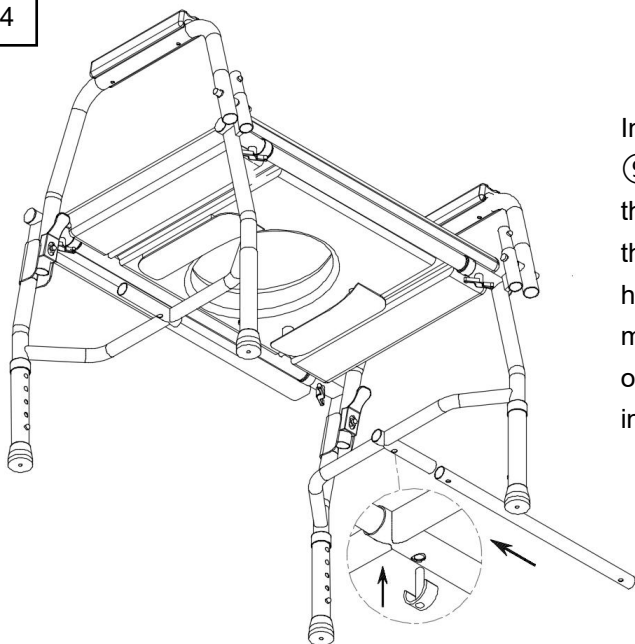


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

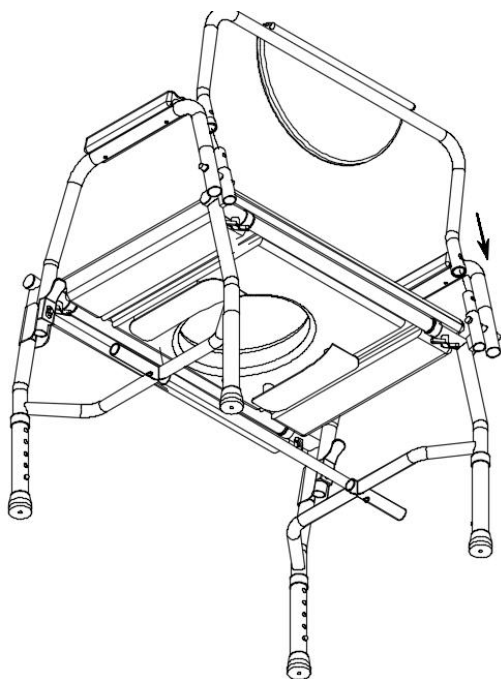

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

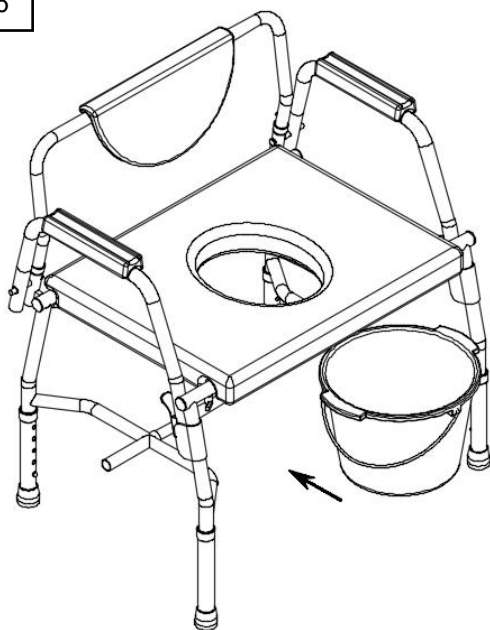

Place the pail⑤ through the front of the seat frame.

7


(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

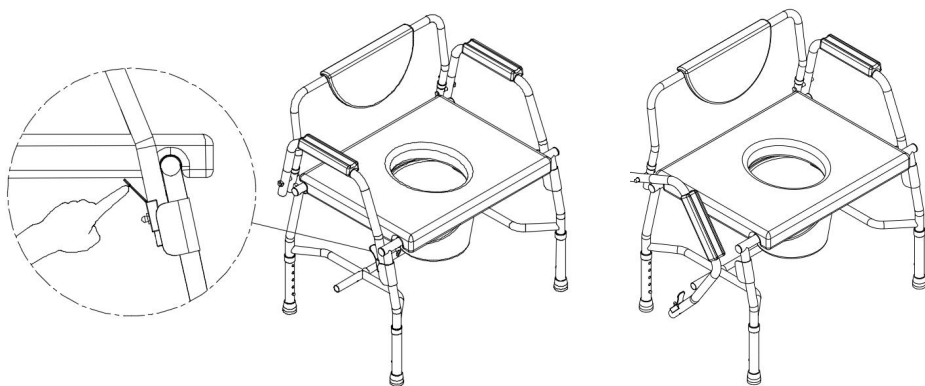




8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

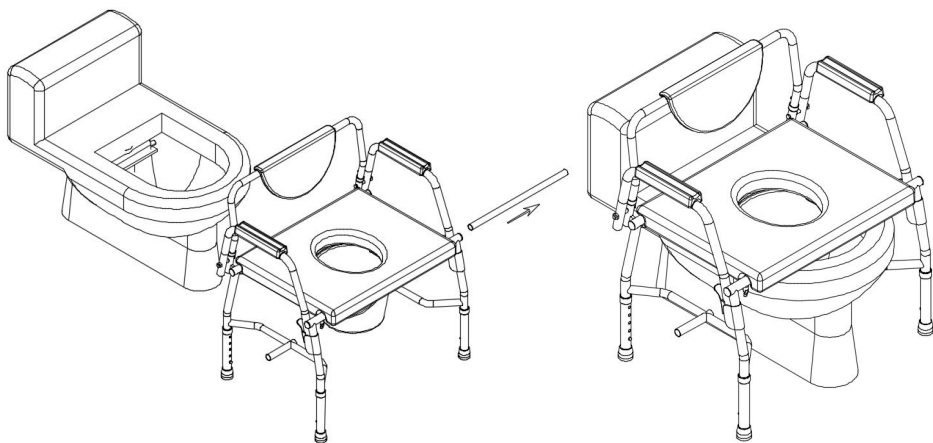

9

Toilet height adjustment, press the marble to pull the legs out and so on.

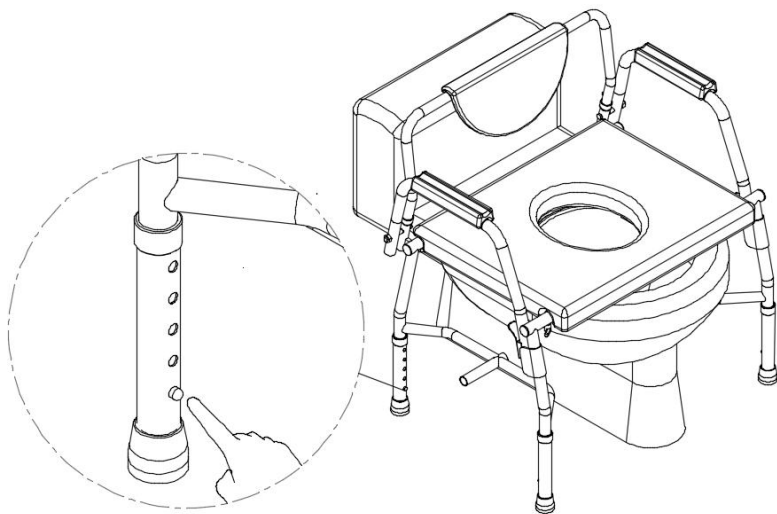

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



**VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**

# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR®

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.

NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2




# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

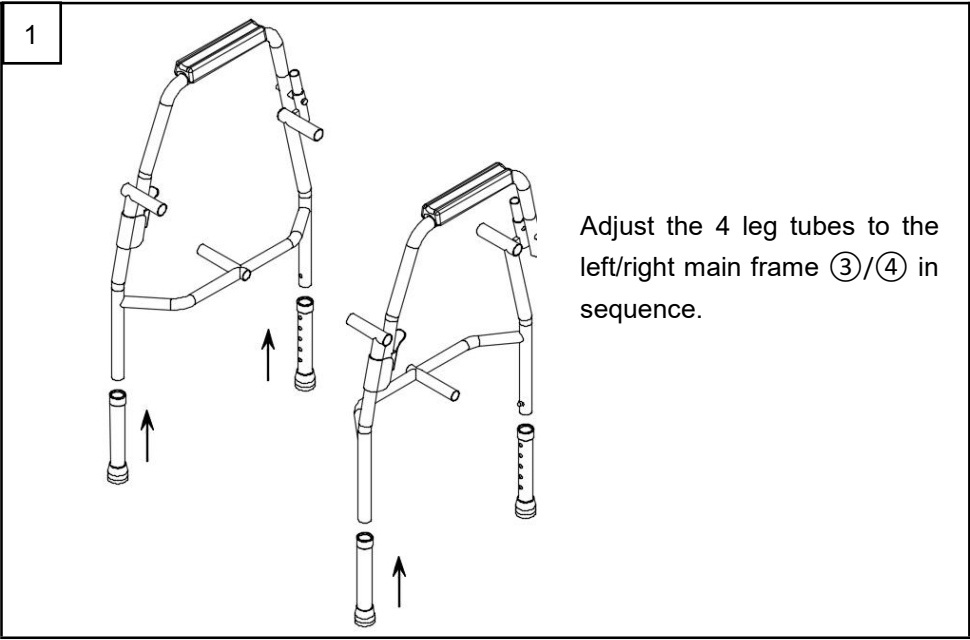

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

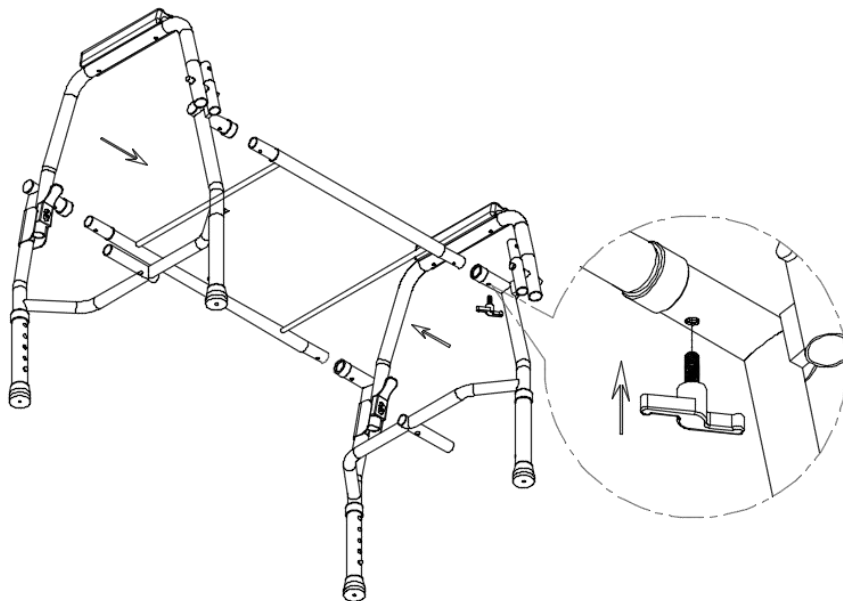


3

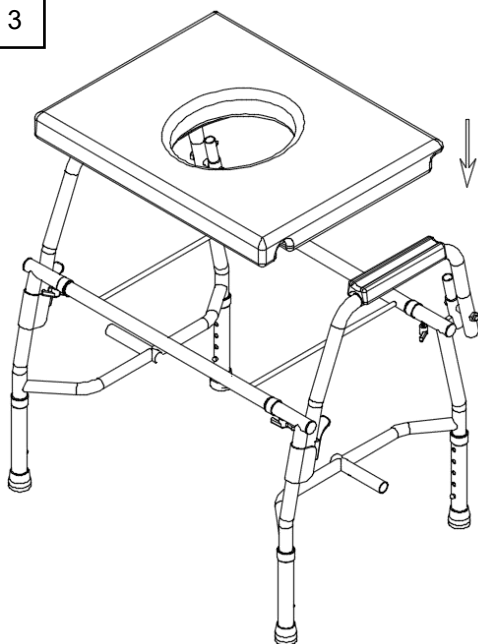


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

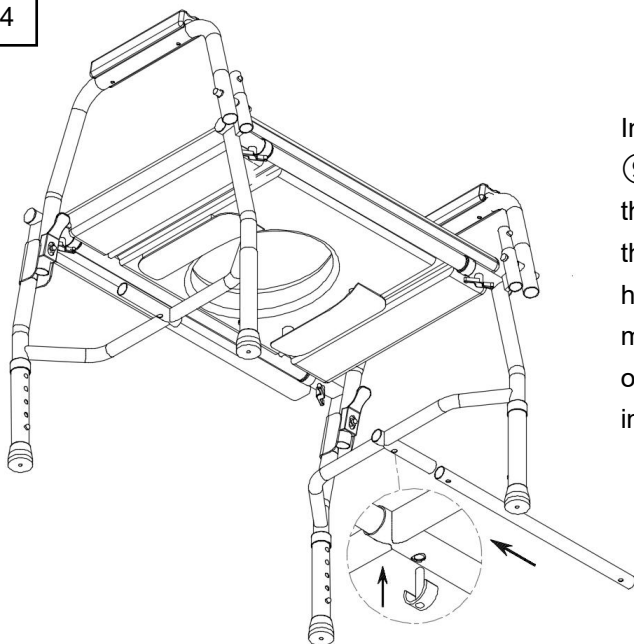


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

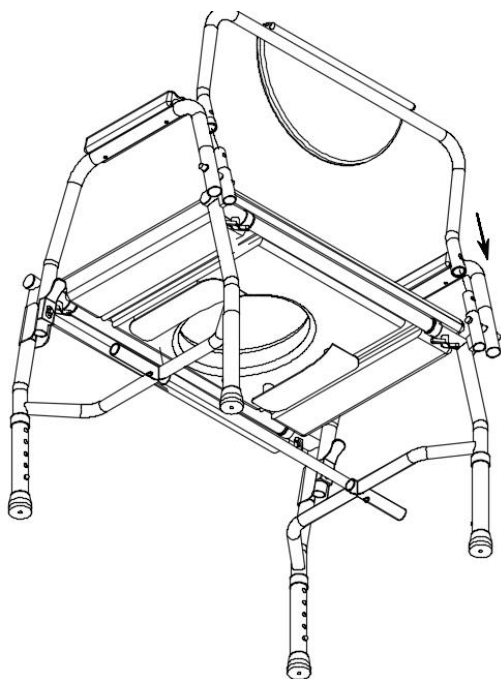

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

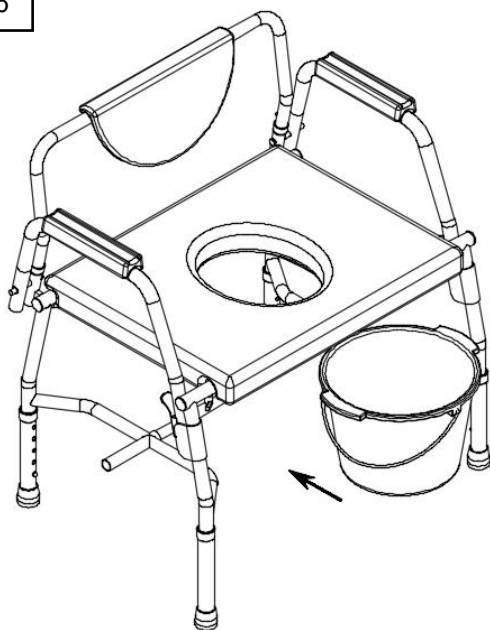

Place the pail⑤ through the front of the seat frame.


7

(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

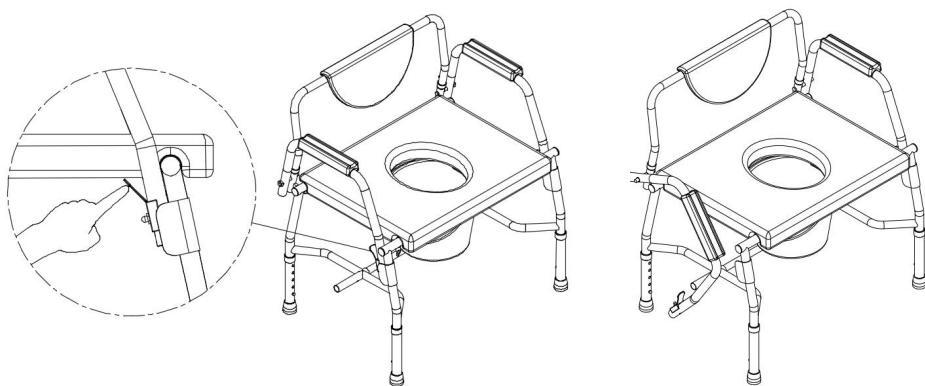


8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

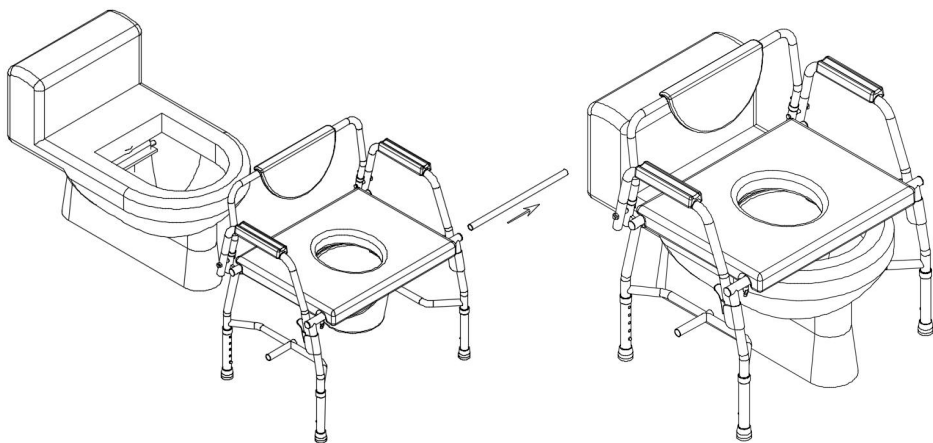

9

Toilet height adjustment, press the marble to pull the legs out and so on.

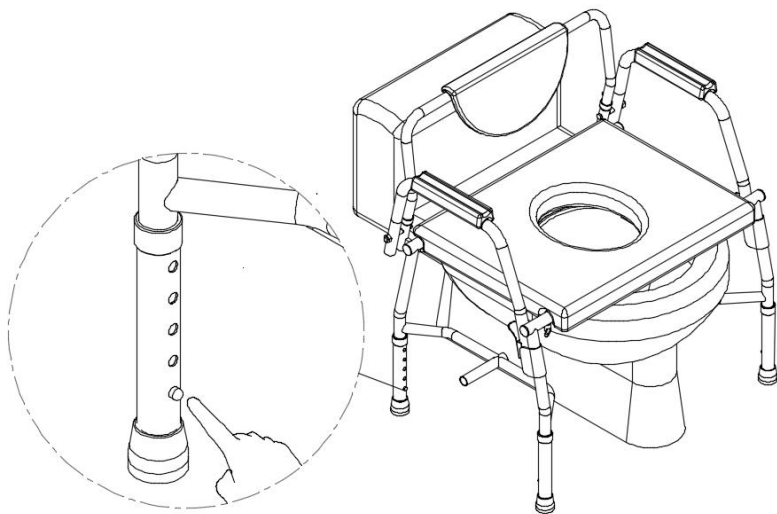

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

Technical Support and E-Warranty Certificate [www.vevor.com/support](http://www.vevor.com/support)

## **COMMODE**

**MODEL:FBL740135**

We continue to be committed to provide you tools with competitive price.

"Save Half", "Half Price" or any other similar expressions used by us only represents an estimate of savings you might benefit from buying certain tools with us compared to the major top brands and does not necessarily mean to cover all categories of tools offered by us. You are kindly reminded to verify carefully when you are placing an order with us if you are actually saving half in comparison with the top major brands.

# VEVOR®

TOUGH TOOLS, HALF PRICE

## COMMODE

MODEL:FBL740135



### NEED HELP? CONTACT US!

Have product questions? Need technical support? Please feel free to contact us:

**Technical Support and E-Warranty Certificate**  
**[www.vevor.com/support](http://www.vevor.com/support)**

This is the original instruction, please read all manual instructions carefully before operating. VEVOR reserves a clear interpretation of our user manual. The appearance of the product shall be subject to the product you received. Please forgive us that we won't inform you again if there are any technology or software updates on our product.

## **WARNING:**

Read the manual completely to avoid harm, product damage, or warranty avoidance. Seek professional help if you encounter discomfort, pain or worsening symptoms. If necessary, use supervision in order to assemble and use this product correctly and safely. Do not exceed the weight limit.

Regularly check for secure assembly and contact support if in doubt. Ensure the product's legs are even and locked before use, and discontinue usage if there are signs of wear, damage, or missing parts. The product is to be used on flat, stable surfaces. Do not disassemble if not necessary, as it might compromise the longevity of the product. Do not modify the product unless specified in the manual.

## **Physiotherapist**

1. Before first use, adjust the height and the width of the rail to your toilet.
2. Back up to the toilet with your assistive device (if available) until the back of your legs are touching the toilet.
3. Reach back for the rail, hold firmly, and slowly lower yourself into a seated position on the toilet.
4. To return to a standing position, place your hands on the rails firmly and push yourself up into a standing position.
5. Once you are standing, gradually let go of the rails, and only then, grab the handle of your assistive device (if available).











## **IMPORTANT**

1. Don't exceed the maximum weight capacity.
2. Use on stable surfaces only.
3. Regularly inspect for signs of wear, damage, or loose parts.
4. Clean regularly using a mild detergent and warm water, rinse off any soap residue. After cleaning, dry thoroughly.
5. Before use, confirm with your healthcare provider that the product meets your specific needs. The following guidelines are not a substitute for medical advice.

## **SAVE THESE INSTRUCTION**

## PART LIST

When unpacking this product, check to make sure the parts listed below are included and carefully inspect for any damage that may have occurred during transit. If any part is missing or damaged, do not attempt to assemble or use the product.


NO	PICTURE	PART NAME	QTY	NO	PICTURE	PART NAME	QTY
①		Seat Frame	1	⑥		Backrest	1
②		Seat	1	⑦		Flat Knob	4
③		Left Main Frame	1	⑧		C-Clip	2
④		Right Main Frame	1	⑨		Connection Tube	1
⑤		Pail & Splash Shield & Lid	1	⑩		Foot Mats (*Gifts)	2

# PRODUCT PAREMETERS


Model	FBL740135
Seat Measures (L×W)	470×590mm/18.5"×23.2"
Seat Height	500-620mm/19.7"-24.4"
Seat Rated Load	454kg/1000lbs

## INSTALLATION AND OPERATION INSTRUCTIONS


### 1. Installation Procedures

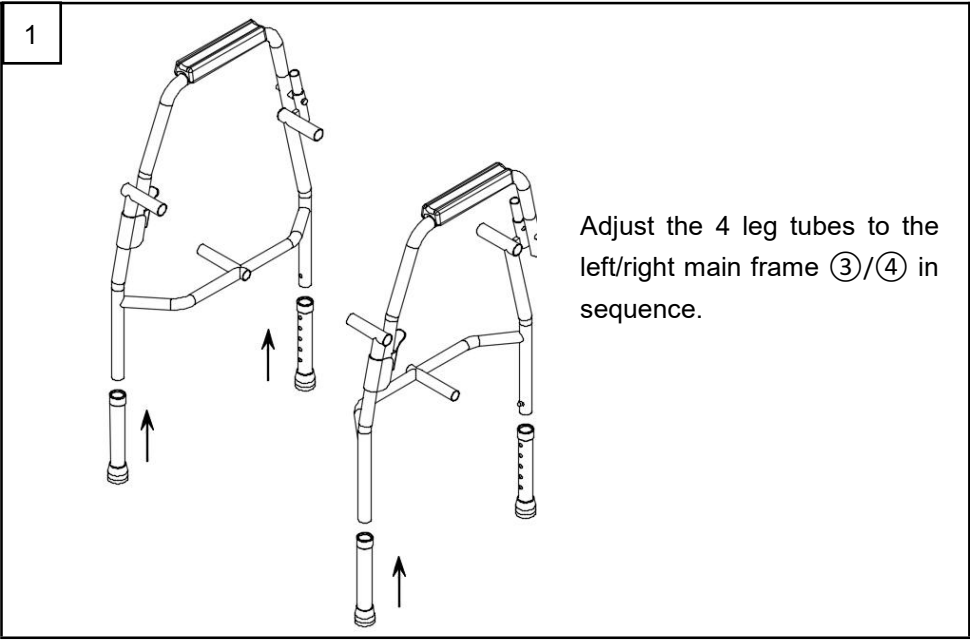

- 2 Insert the assembled left/right main frame③/④ in line with the tube ports of the seat frame①, and then lock it with the flat knob⑦.

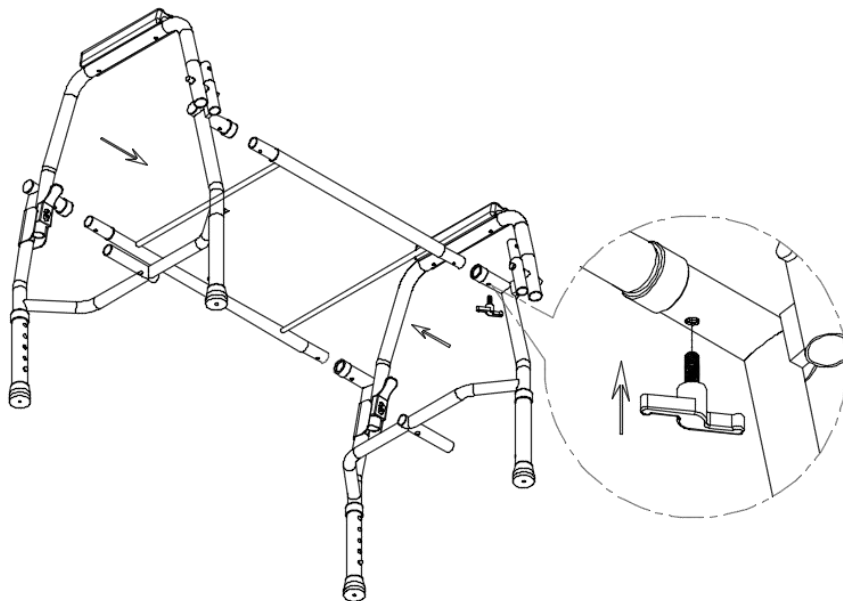


3

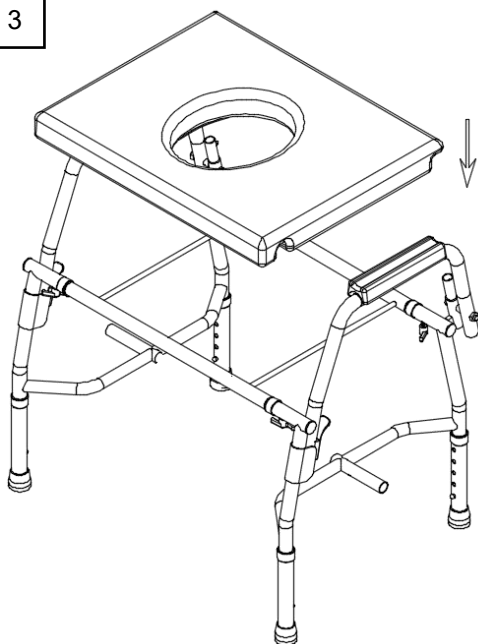


Install the seat plate, the slot on the back of the seat plate is aligned with the seat frame and then pressed down, the bottom of the seat plate buckle and the small tube of the seat frame buckle steady.

4

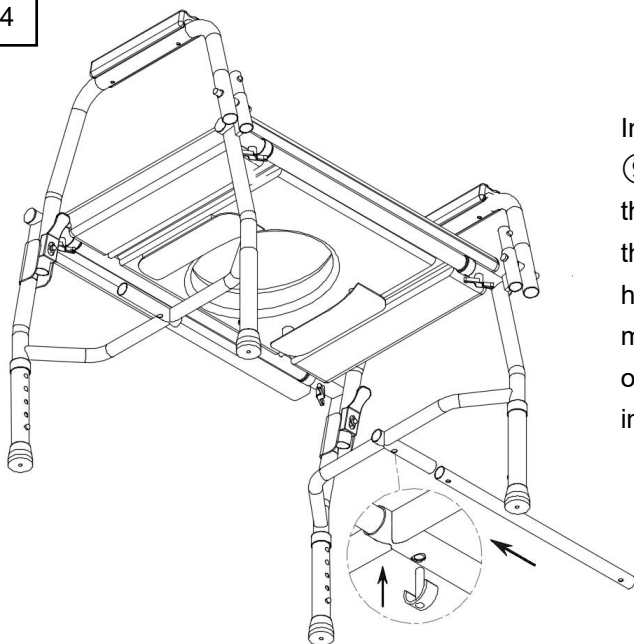


Insert the connecting tube ⑨ laterally on the side of the main frame mouth so that the connecting tube hole is aligned with the main frame connecting outer tube hole, and then insert the C-clip ⑧.

5

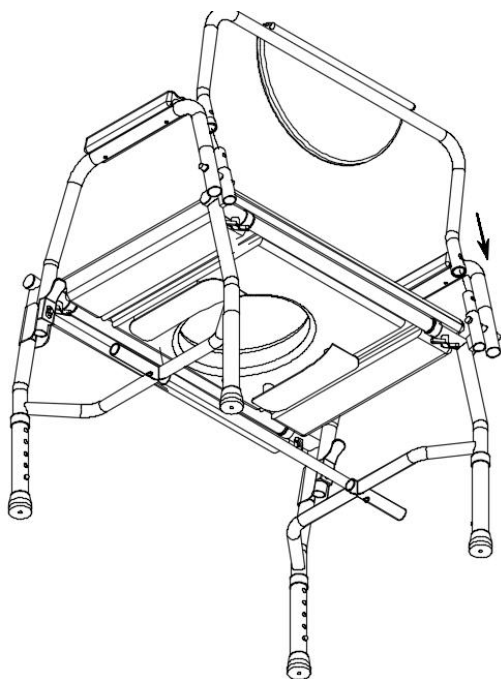

Install the backrest, (as shown in the picture) align the backrest with the main frame mounting tube, press the marble and insert the backrest, the marble pops out in the backrest hole and locks.


6

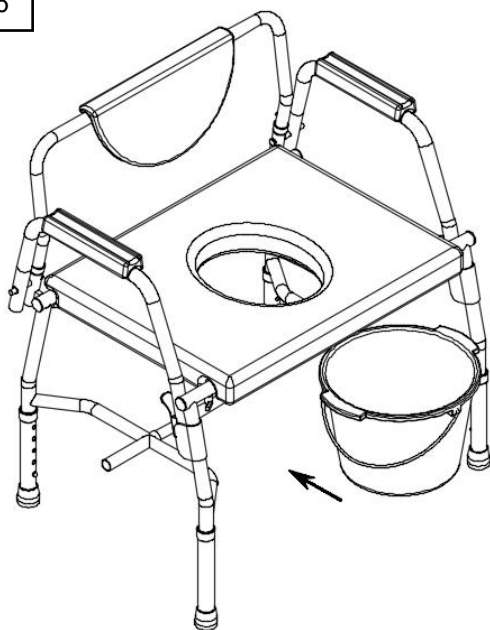

Place the pail⑤ through the front of the seat frame.

7


(Armrest Removal) As shown in the figure: press the armrest fixing button to lower the armrest.

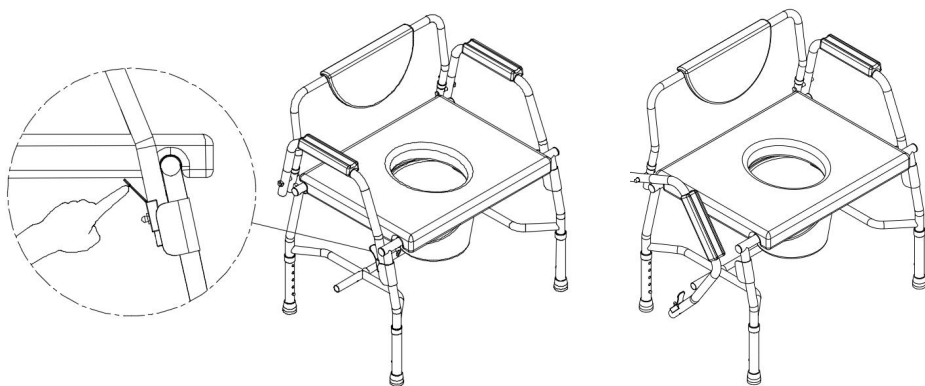




8

Instructions for use: Before putting into the toilet, remove the C-clip, take the connecting tube out from the side, and then put it into the toilet for use.

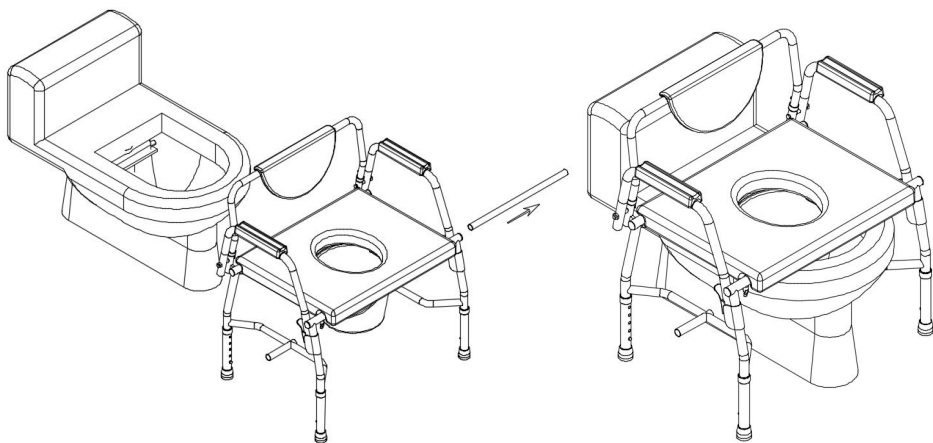

9

Toilet height adjustment, press the marble to pull the legs out and so on.

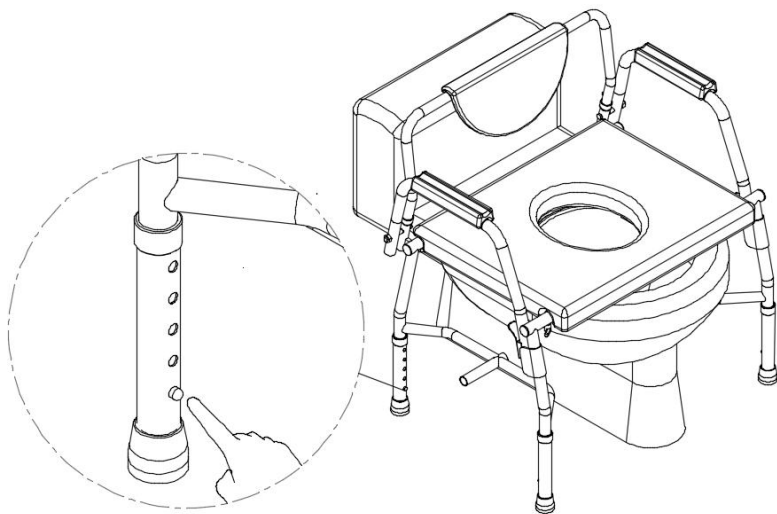

## **Zhongshan Bliss Medical Instrument Co., Ltd**

**Address:** 3-6F & 7F-1, No. 63, Tongxing East Road, Yumin Community  
Xiaolan, Zhongshan, Guangdong, 528414, CHINA



Pooledas Group Ltd  
Unit 5 Albert Edward House,  
The Pavilions Preston, United Kingdom  
pooledas123@gmail.com  
01772418127



SHUNSHUN GmbH  
Römeräcker 9 Z2021,76351  
Linkenheim-Hochstetten, Germany  
euvertreter@gmail.com  
+49 1727041930

**Made In China**



# **VEVOR<sup>®</sup>**

**TOUGH TOOLS, HALF PRICE**

**Technical Support and E-Warranty Certificate**

**[www.vevor.com/support](http://www.vevor.com/support)**