
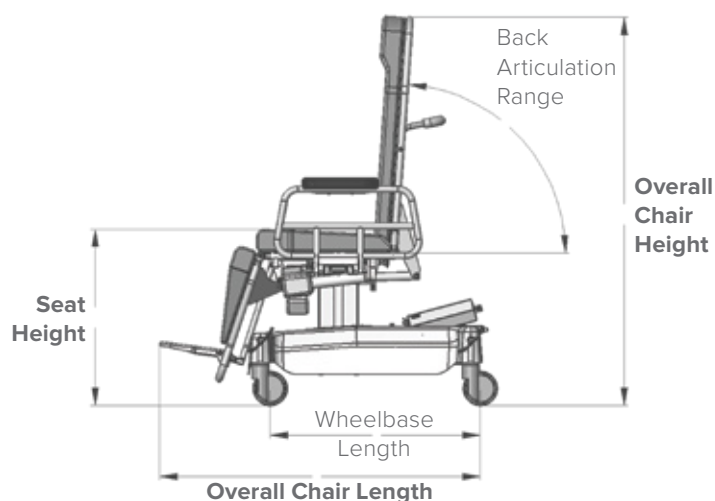


*VFSS STRETCHER-CHAIR

SPECIFICATION DESCRIPTION

SPECIFICATION MEASUREMENT


Maximum Patient Weight	350 lb. (159 kg.)
Seat Height, Low	25.1 in. (64 cm.)
Seat Height, High	33 in. (83.82 cm.)
Seat Cushion Height, Front (tapered)	3.25 in. (8.26 cm.)
Seat Cushion Height, Back (tapered)	2.25 in. (5.08 cm.)
Back Cushion Height	33 in. (83.82 cm.)
Seat Width	24 in. (61 cm.)
Back Width (no extension)	15 in. (38 cm.)
Back Width (w/ optional extension)	24 in. (61 cm.)
Radiolucent Window (width x height)	13 in. x 26 in. (33 cm. x 65 cm.)
Overall Width (rails up)	30.5 in. (77.47 cm.)
Patient Surface Length (standard)	77 in. (195.58 cm.)
Patient Surface Length (w/ manual folding footrest)	70.4 in. (179 cm.)
Overall Chair Height, Low	55.5 in. (141 cm.)
Overall Chair Height, High	63 in. (160 cm.)
Backrest Articulation	0° - 86°
Side Rail Height When Up (seat pan to rail top)	10.88 in. (27.64 cm.)
Side Rail Length	21.1 in. (54 cm.)
Wheelbase (length x width) (standard)	30 in. x 20 in. (76 cm. x 51 cm.)
Wheelbase (length x width) (S short option)	26 in. x 20 in. (66 cm. x 51 cm.)

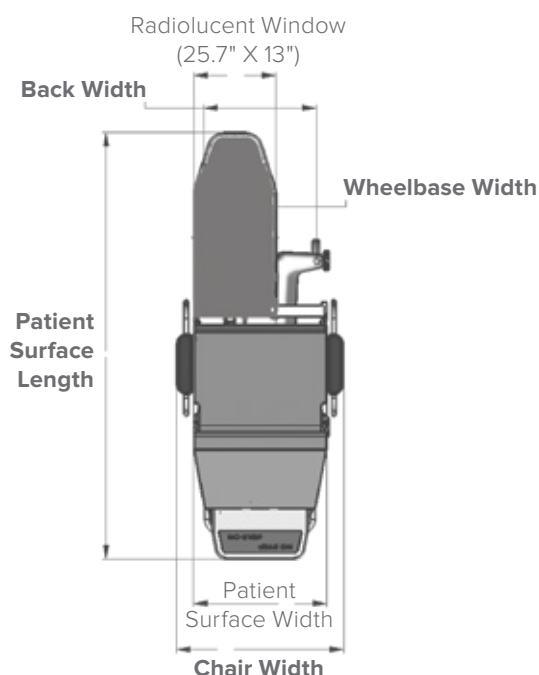

TMM3 STRETCHER-CHAIR SPECIFICATIONS


CHARGING SYSTEM	POWER SPECIFICATION
Input, Volts	100 VAC - 240 VAC
Input, Current	1.0 A (max)
Input, Frequency	50 HZ / 60 HZ
Output	+24 DC 1.4 A
Maximum Power	36 W
Battery	24V – 4.5Ah Sealed Lead Acid
Mode of Operation	1 Min Load / 9 Min Rest

PENDANT FUNCTIONS

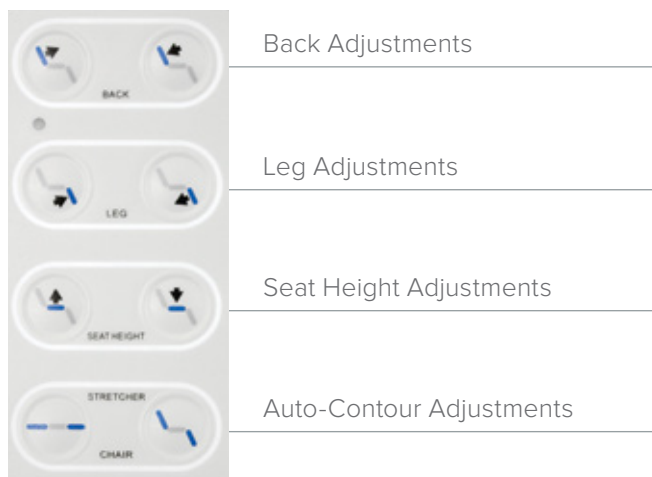

*VFSS = Video Fluoroscopy Swallow Study

NOTE: Winco Mfg., LLC reserves the right to revise specifications without notice.



CONTACT US

To arrange a demonstration or to speak with one of our associates, please feel free to contact us at:
800-237-3377 | WincoMfg.com | 5516 SW 1st Lane, Ocala, FL 34474 | Info@WincoMfg.com