


# **QUICK NOTES**

#### TMM5 PLUS SURGICAL STRETCHER-CHAIR



#### 1. ARTICULATING HEADPIECE ADJUSTMENTS

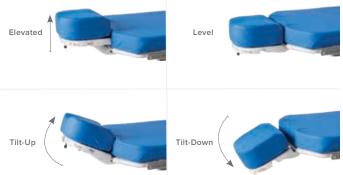

#### Raising / Lowering the Headpiece

Support the headpiece with your left hand, squeeze the right red lever and adjust height to desired level.

# Adjusting the Slope of the Headpiece

Support the headpiece with your right hand, squeeze the left red lever and adjust to desired angle.





MAXIMUM PATIENT WEIGHT IS 500 lbs (227 kg.)

### 2. SIDE RAIL - LOWERING/RAISING



#### Lowering the Side Rail

Grasp the top of the side rail and push slightly inward while pulling out the Red release tab at the bottom of the rail.

#### Stowing the Side Rail

Lower the rail into the down position.



#### Raising the Side Rail

Lift the side rail until it is in the up position. The Red release tab will engage (lock) automatically.



After raising, pull on side rail to ensure it is securely locked.

### 3. BACK SECTION QUICK RELEASE



#### Location

The (Red) quick release lever is located under the seat on the patient's right side.

#### **Activating the Quick Release**

Pull the Red lever out towards the side rail. When weight is applied, the back section will drop until the lever is released.



Intended for EMERGENCY purposes ONLY.

#### 4. CASTER BRAKE OPERATION



#### **Brake Mode**

Activate the braking system by pressing down on the red end of either brake pedal.



This mode prevents all four casters from swiveling and all four wheels from spinning.



#### **Neutral Mode**

Activate the neutral mode by placing either brake pedal into a horizontal orientation.



This mode allows all four casters to swivel and all four wheels to spin freely.



#### Steer Mode

Activate the steer-locking system by pressing down on the green end of either brake pedal.



caster parallel to the base but allows the other three casters to swivel and all four wheels to spin freely.

#### 8. EIGHT BUTTON PENDANT

#### **Pendant Storage**

To prevent damage, the pendant may be stored at various locations on the chair when not in use.



Pendant is NOT INTENDED ! CAUTION FOR PATIENT USE.

#### **Back Adjustment**

The first row of buttons controls the angle of the back section. Press the left button to raise the chair back. Press the right button to lower the chair

#### Leg Adjustment

The second row of buttons controls the angle of the leg section. Press the left button to raise the leg section. Press the right button to lower the leg section.

#### **Seat Height Adjustment**

The third row of buttons controls the seat height. Press the left button to raise the seat. Press the right button to lower the seat.

## **Auto-Contour Adjustment**

The fourth row of buttons controls the simultaneous actuation of the leg and back sections. Press the left button to place the chair in a stretcher position. Press the right button to place the unit into the chair position.



This mode locks front right

#### 5. BATTERY PACK ("B" OPTION) INSTALLATION AND REMOVAL



#### **Battery Pack Removal**

Grasp the battery pack's integrated handle and lift up until locks disengage then pull the battery away from the mounting bracket.



#### Installing the Battery Pack

Place the two circular pins located on the back of the battery pack into the square openings on the battery mounting bracket. Once the pins are aligned, slide the battery pack down until the pins lock into place.



To maintain an optimum charge, Winco recommends charging your battery every 2-3 days.

#### 6. PUSH BAR OPFRATION



#### Lowering the Push Bar

Grasp the push bar handle while pulling out the Red release knob and lower the push bar.

#### Raising the Push Bar

Lift up on the push bar handle until the Red release knob engages (locks).

#### 7. AUTO-EXTENDING FOOTREST



### Storing the Footrest

Lift the end of the footrest until it engages in the stored, upright position. The footrest should be stored in this position when not being used.

#### Lowering the Footrest

Push down on the footrest to lower for use.



WARNING Do not stand or sit on foot rest.

## **A**WARNING

PATIENT MUST ENTER / EXIT FROM THE SIDE WITH THEIR BODY WEIGHT CENTERED OVER SEAT SECTION.

**PATIENT INGRESS / EGRESS SHOULD** ALWAYS BE MADE WITH THE UNIT IN AN **UPRIGHT-CHAIR POSITION WITH CASTERS** LOCKED.



For additional assistance, please contact us at:

800-237-3377 | 352-854-2929 5516 SW 1st Lane, Ocala, FL 34474 WincoMfg.com