User Manual
Meissa OT

Rehabilitation robot for upper limbs



Read carefully before use

Applies to:

Meissa OT Pro

Meissa OT Ultra

Gliwice, Poland rev. 10

CE 2274

Date of first publication of the User Manual: 2023-03-30

1. We are there for you!

Thank you for ordering your Meissa OT

and welcome to our family!

At **EGZO**Tech, we truly believe that **great user experience isn't just about having great products, but also reliable support, constant development, and understanding the needs of people using our products** - patients and therapists alike. We truly believe that together, we can change the future of healthcare and physiotherapy!

The next steps will **empower your therapy with Meissa OT!**

To learn more about **Meissa OT**, visit the following:

Our YouTube page for videos!

https://youtube.com/EGZOTech

If you're having unexpected operation or events, issues, serious incidents or any trouble with your Meissa OT, please contact us at the following:

Our Service Desk page:

https://service.egzotech.com

Other direct contact information:

support@egzotech.com
https://egzotech.com
+48 32 750 49 45
EGZOTech Sp. z o.o.
Romualda Traugutta 6H
44-100 Gliwice, Poland

We provide additional resources for education, support, maintenance and webinars.

Feel free to check **EGZO**Tech Courses available at https://www.egzotech.com/en/knowledge-base/.

Any serious incident related to **Meissa OT** has to be reported to **EGZO**Tech and the competent authorities of the country. Please inform us by sending a message to the address safety@egzotech.com.

2. Quick setup guide

We honestly understand that no one likes long instructions. That's why we want to streamline this process. Check out the website below with a video tutorial:

Don't like reading? Check out our video tutorials available on the website https://www.egzotech.com/en/knowledge-base/.

2.1 Safety

Remember, **Meissa OT can be dangerous if used incorrectly!**

Do not start using Meissa OT before reading this User Manual, especially **7. Warnings and basic safety** chapter.

2.2 Unboxing

Meissa OT is delivered with all the ordered accessories in a package. On initial delivery, **please check the contents to confirm that everything you've ordered has been properly delivered.** Remember to remove Meissa OT with accessories from the packaging and remove all packaging items before starting up.

Use your device only in a permissible temperature range (10-40℃). Before you start working with Meissa OT, the device should be allowed to reach ambient temperature.

Time required for reaching the ambient temperature 20℃ from the minimum permissible storage temperature is 1 h.

Time required for reaching the ambient temperature 20℃ from the maximum permissible storage temperature is 2 h.

2.3 Starting up your Meissa OT

Step 1: Mount the device to the tabletop. Make sure the device is securely attached and there is no risk of the device shifting during exercise.

Step 2: When the device is connected to the AC power network press the main activation button marked on the picture below. Meissa OT will automatically turn ON as well as its tablet which will provide the user with further instructions.



The manufacturer recommends that **Meissa OT device be connected directly to the mains socket** (not through an extension cord) or directly to the power network. However, if this is not possible, ensure that any **extension cord used is grounded** and **as short as possible** (not applicable in home healthcare environment).

Be aware that Meissa OT is designed for permanent installation if used in a home healthcare environment; therefore, it is essential to review the information provided in section **6.6 Use in a home healthcare environment**.

Step 3: Create a new clinic or log in. Pressing the "sign up" text will redirect you to a clinic creating form, and then log in.

Step 4: The device is ready to use. Create a new patient profile or choose an already existing profile from the patients list. After creating a new patient profile or choosing an existing one, the exercise selection screen will appear.

Step 5: Select the required exercise from the list. For every exercise, Basing will be required. Note that further instructions for steps from 6 to 12 are shown on the tablet and depend on chosen exercise. Exercise-specific steps and details may also appear.

Step 6: Set the required parameters.

Step 7: Choose the trained side - left or right.

Step 8: Mount the required extension. If it has not been mounted yet, the application will notify you, and guide through the extensions.

Step 9: Set the axis of the device with the requirements. Each axis of rotation is set independently.

Step 10: Ensure proper patient position during exercise. It is recommended to perform the exercises in the anatomical position. For this reason, it is recommended to use a height-adjustable table and an arm support accessory.

Step 11: Set the Range of Motion:

- Measure Passive Range of Motion (ROM) with Meissa OT by performing maximum passive movement of the patient's hand with an external aid (clinician or therapist).
- Measure Active Range of Motion (ROM) with Meissa OT by having the patient perform an active hand movement (without external assistance).

Step 12: The device is ready to use.

Congratulations! Your Meissa OT is ready to perform a training! Before you start, we strongly advise you to read the rest of this manual and watch our YouTube videos to learn how to use Meissa OT to best efficiency. Let us know what your experience is on Facebook!

2.4 Accessing the Application

Step 1: Visit the main page of the application.

Step 2: Create a new patient profile or choose an existing patient to start performing exercises.

2.5 Finishing your work with Meissa OT


Step 1: Disable electrical stimulation (Meissa OT Ultra only) and end programs within the application first.



Never grab the electrodes during electrical stimulation (Meissa OT Ultra only). Always ensure that the stimulation is disabled first.


Step 2: Turn off the main power button. Disconnect Meissa OT from the power source by unplugging the AC cable or, in the case of permanent installation in a home healthcare environment, the AC cable should only be disconnected by authorised personnel.

Step 3: Disconnect all the electrodes and cables from the patient's body (Meissa OT Ultra only). Grab the cable snap (red mark located on the right and left side) and pull it off from the electrode by giving some force to detach it.

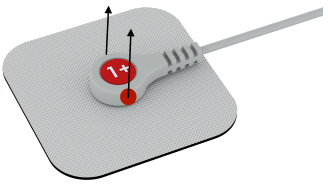

Step 4: Disconnect the electrode cables from the cable HUBs (Meissa OT Ultra only).

Step 5: Disconnect the electrode cable from the device by pressing the latches on both sides of the cable connector and pulling it away from the connector port.

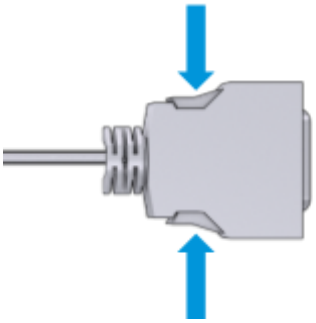

Step 6: Put everything in the transportation box.

3. Table of contents

1. We are there for you! 3

2. Quick setup guide 4

2.1 Safety 4

2.2 Unboxing 4

2.3 Starting up your Meissa OT 4

2.4 Accessing the Application 6

2.5 Finishing your work with Meissa OT 6

3. Table of contents 7

4. Where to get this manual? 11

5. What is Meissa OT 11

6. User responsibilities 13

6.1 Indications for use 13

6.2 Intended users 14

6.3 Contraindications 15

6.4 Facility responsibilities 17

6.5 Internet connection 17

6.6 Use in a home healthcare environment 18

6.6.1 Guidelines for installing devices in a home environment 18

7. Warnings and basic safety 21

7.1 General safety consideration and precautions 21

7.2 Clinical safety 23

7.3 Electrical safety and electromagnetic compatibility 24

7.4 Electrical stimulation safety, including TENS (Meissa OT Ultra only) 26

7.5 Mechanical safety 28

7.6 Multiple use precautions and consumables 29

7.7 Biological safety 30

7.8 Environmental safety 30

7.9 Software safety and cybersecurity 31

7.10 Lifetime 31

7.11 Annual maintenance 32

7.12 Risk and benefits 32

8. How to work safely with Meissa OT? 33

8.1 Why this user manual is so important 33

8.2 Labelling 33

8.3 Software Version Identification 34

8.4 Symbols 34

8.5 Accessories symbols 37

9. What will I find in the package? 38

9.1 Meissa OT 38

9.1.1 Extensions 38

9.1.1.1 Extension for elementary movement 38
9.1.1.2 Occupational therapy extensions 39
9.1.2 AC Power Cable 39
9.1.3 Table mounting clamp 40
9.2 EMG/EMS cable - 1 pc. (Meissa OT Ultra only) 40
9.3 Electrodes for surface electromyography (Meissa OT Ultra only) 42
9.4 Electrodes for electrostimulation (Meissa OT Ultra only) 42
9.5 Transport Box 43
9.6 Electric Table 44
9.6.1 Electric Table use and adjustment 46
9.6.2 Troubleshooting 47
9.7 Arm Support 48
9.7.1 Arm Support assembly 50
9.7.2 Arm Support use and adjustment 53
10. Basic information about Meissa OT 56
10.1 How is Meissa OT built 56
10.2 Technical Specifications 58
10.3 Platform - How to mount/dismount Meissa OT to/from the worktop 59
10.4 Head - Adjustment of Meissa OT in the vertical and horizontal planes 61
10.5 Tablet holder - Adjustment of the tablet position 62
10.6 LED Ring - Visual notification 63
10.7 Sound notification 64
10.8 Typical issues 64
10.9 Emergency stop push buttons 65
11. Extensions 67
11.1 What kind of extensions do I have? 67
11.2 Plug in/out your extension 67
12. Electromyography (Meissa OT Ultra only) 69
12.1 How it works 69
12.2 Lead wires and channels for EMG 69
12.3 Electrodes 70
12.4 EMG Electrode placement and configuration 70
13. Electric stimulation (Meissa OT Ultra only) 72
13.1 Basics of electrical stimulation 72
13.2 Lead wires and channels for EMS 72
13.3 EMS Electrode placement and configurations 72
13.3.1 EMS Programs - Electrode Arrangement 73
13.3.2 EMG - Electrode Arrangement for EMG-triggered EMS Programs 74
13.4 Electrical stimulation modes 74
14. Notifications, Information, Errors, and Warnings displayed by the Software 77
14.1 Dialog window 77
14.2 Pop-up notification 78

14.3 Configuration or exercise screen 78
14.4 Inline text or checkmark notification 93
14.5 Errors 93
14.6 Warnings 93
14.7 Notifications 94
14.8 Reports 95
14.8.1 Saving a report to a USB drive 97
15. Software 99
15.1 How to launch the application 99
15.2 Registration 99
15.3 Signing in 99
15.4 Clinic's profile 99
15.5 Patient's profile 99
16. How to set up a training program 100
16.1 What exercises can I perform? 102
17. Programs Overview 103
17.1 Continuous Passive Motion (CPM) 103
17.1.1 CPM 103
17.1.2 CPM Force 103
17.1.3 CPM + EMS (Meissa OT Ultra only) 103
17.1.4 CPM + EMG (Meissa OT Ultra only) 103
17.1.5 CPM + EMG + EMS (Meissa OT Ultra only) 104
17.2 Continuous Active Motion (CAM) 104
17.2.1 CAM Isokinetic 104
17.2.2 CAM Torque 104
17.2.3 CAM Turn Key 104
17.2.4 CAM Games 104
17.2.4.1 CAM Game “Cosmic Mission” 105
17.2.4.2 CAM Game “Dream Drive” 105
17.2.4.3 CAM Game “Ocean Paradise” 105
17.2.4.4 CAM Game “Cat Crunch” 106
17.2.4.5 CAM Game “Doggo Nom” 106
17.2.4.6 CAM Game “Rope-Nope” 106
17.2.4.7 CAM Game “Elevator Express” 106
17.2.4.8 CAM Game “Parkour Fever” 107
17.3 EMS Programs settings (Meissa OT Ultra only) 107
17.3.1 EMS programs details 107
17.3.2 Custom EMS Program settings 108
17.4 Typical use cases 108
18. Miscellaneous 110
18.1 How to identify your Meissa OT or accessories 110

18.2 Behaviour of Meissa OT 110
18.3 Description of user maintenance responsibility 111
18.4 Software auto updates 111
18.5 Electrical isolation information 111
18.6 Expected product service life 112
18.7 Storage and transportation instructions 112
18.8 How to safely dispose of the device 113
18.9 Warranty 113
18.10 Manufacturer's service obligation 114
19. Cleaning 115
20. Data protection 119
20.1 End user license agreement (EULA) 119
20.2 Data retention 119
21. Declaration of Conformity and compliance statements 120
21.1 Declaration of Conformity 120
21.2 Manufacturer's declaration – electromagnetic emissions 120
21.3 Manufacturer's declaration – electromagnetic immunity 120
21.4 Recommended separation distances between portable and mobile RF communications equipment and Meissa OT 122
21.5 RF Radio Regulatory Statement 123
22. Meissa OT permanent installation protocol - home healthcare environment only 124

4. Where to get this manual?

Before use, always be sure to check whether this manual corresponds to the version of Meissa OT you are using. **EGZO**Tech is not responsible for any misuse that may arise due to using an outdated version of this manual.

The latest version of the User Manual is always accessible on http://www.egzotech.com, and can also be requested from the helpdesk.

5. What is Meissa OT

Meissa OT is a multi-use upper limb rehabilitation robot - rehabilitation exercise device intended for medical purposes of rehabilitation and physiotherapy, including therapy and evaluation of patient's state.

Meissa OT Pro has two main functions:


- Continuous passive motion,
- Continuous active motion.

Meissa OT Ultra has the above and additionally:

- Electromyography measurement and biofeedback,
- Electrical muscle stimulation.

The main value propositions are:

- EMG-Triggered movement, Functional Electrical Stimulation and EMG-Triggered electrical stimulation (Meissa OT Ultra only),
- Extensions for elementary movements of the hand and fingers,
- Easy to use with quick and simple exchange of extensions during training sessions,
- Device mounted to the tabletop with easy adjustment of the axis of movement for the patient,
- Pre-set therapeutic protocols and therapeutic games,
- Programs for home therapy.

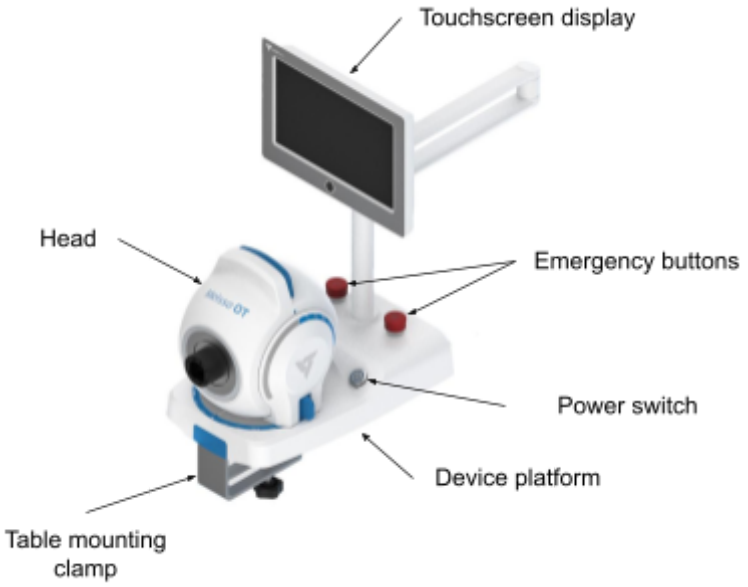

Main parts of Device:

- Device platform - with mounting system, is fixed to the tabletop,

- Device working part (head) - can be rotated in relation to the platform horizontally in a range of -90° to 90° and vertically in the range of 0° to 90° in 15° increments,
- Touchscreen display,
- Table mounting clamp,
- Extensions set for occupational therapy,
- Extensions set for elementary movements.

The therapy is conducted by evaluation of a range of motion and/or force, and/or locating EMG or EMS electrodes (Meissa OT Ultra only) and selecting an evaluation program or exercise. The device is intended to conduct rehabilitation procedures in a sitting or standing position. The robot is controlled using a touchscreen equipped with proper software dedicated for the device.

The device shall be mounted to the table top.



Meissa OT is an automatic physiotherapy device. **Misconfiguring the training parameters**, especially electrostimulation parameters, range of motion, maximal applied torque and maximal speed **can lead to injuries!**

If the document refers to Meissa OT, it should be understood as applying to both Meissa OT Pro and Meissa OT Ultra models.

6. User responsibilities

6.1 Indications for use

Indications:

Meissa OT is a multi-use upper limb rehabilitation robot - rehabilitation exercise device intended for medical purposes of rehabilitation and physiotherapy, including therapy and evaluation of patient's state.

Meissa OT is intended for the following:

- Physiotherapy and occupational therapy to:
    - Increase muscle strength;
    - Increase the limb range of motion;
    - Increase coordination;
    - Relaxation of muscle spasms;
    - Relearn voluntary motor functions of the extremities;
    - Muscle re-education and relaxation;
    - Relief and management of pain;
- Physiotherapy and occupational therapy using electrical stimulation (Meissa OT Ultra only) to:
    - Increase the limb range of motion (using EMS);
    - Relaxation of muscle spasms with EMS;
    - Muscle re-education and relaxation with EMS;
    - Relearn voluntary motor functions of the extremities with EMS;
    - Increasing local blood circulation;
    - Immediate post-surgical stimulation to prevent venous thrombosis;
    - Prevention or retardation of disuse atrophy;
    - Relief and management of pain with using EMS;
- Rehabilitation assessment to:
    - Evaluate muscle innervation by surface electromyography (Meissa OT Ultra only);
    - Evaluate ranges of motion;
    - Evaluate limb rigidity and spasticity;
    - Evaluate maximum muscle strength;
    - Evaluate fatigability.

This list is not meant to be exhaustive.

Patients:

Patients - especially suffering from the conditions listed in the **6.1 Indications for use** chapter.

Patients are not generally considered users or operators of the device, unless they meet the requirements of a lay operator as defined in chapter **6.2 Intended user**.

Meissa OT is indicated to be used by all groups of patients (over 3 years old), giving consideration to the maximal allowable values provided in the chapter **10.2 Technical Specifications**.

The patient readiness and appropriateness of use, must be individually assessed by the prescribing or supervising clinician. The clinician is responsible for determining whether the child demonstrates sufficient physical and/or cognitive maturity to safely and effectively be a patient of the device. In cases where this cannot be assured, therapy should not be initiated.

Patient groups should be considered among others:

- Low mobility patients (external use) - patients with possibly severely impaired mobility and lack of sensation in their limbs, patients with muscle strength at levels 0-2 on the Lovette's scale, also with difficulties of correct definition of their possible muscle strength due to a huge loss of mobility.
- Non-low mobility patients (external use) - patients with muscle strength from level 3 on the Lovette' scale.

This list is not meant to be exhaustive.

Meissa OT can be used by patients independently, without supervision, as a lay operator. However, in this case, the patient has to be an adult user (at least 18 years old) with at least 8 years of education, be conscious, and understand the risks and safety aspects associated with the use of Meissa OT. In addition, the patient must not have any motor impairments that could hinder the use of the device or their ability to respond appropriately in case of an emergency.

If the patient is a lay operator (the device is used without supervision), the scope of responsibility is the same as that described for the lay operator in chapter **6.2 Intended user**.

The usability of the identification, marking and accompanying documentation intended for the lay operator (patient) is evaluated based on an operator profile that includes a minimum of eight years of education and adulthood.

6.2 Intended users

Meissa OT is intended for two primary user groups:

LAY OPERATORS - adults users (at least 18 years old) with at least 8 years of education. Who understands the risks and safety regarding the use of Meissa OT. Possessing physical capabilities sufficient to perform all device-related tasks without introducing additional risk or compromising usability.

The usability of the identification, marking and accompanying documentation intended for the lay operator is evaluated based on an operator profile that includes a minimum of eight years of education and adulthood.

Meissa OT Pro is for you, to help you achieve the benefits of using Continuous Passive Motion (CPM) and Continuous Active Motion (CAM) motorized movement programs with your therapist, as well as, by yourself in a home and home healthcare environment.

Meissa OT Ultra is for you, to help you achieve the benefits of the combination of electromyography and electrical stimulation used in Continuous Passive Motion (CPM) and Continuous Active Motion (CAM) motorized movement programs with your clinician, as well as, by yourself in a home and home healthcare environment. Feel free to use electromyography biofeedback functionalities (Meissa OT Ultra), as they are considered safe to use in most cases. Remember however to take care while working with Meissa OT (read the safety instructions!). **You need training and consultation from a healthcare professional on how to use Meissa OT safely before you start using it yourself.**

We do expect **patients using Meissa OT without supervision** to be adults (at least 18 years old) with at least 8 years of education. You have to be conscious and understand the risks and dangers of using Meissa OT. You must perform all tasks related to the device without introducing additional risks or limiting usability. If you have any doubts about whether you understand this manual and especially the **7. Warnings and basic safety** chapter, please ask your clinician for assistance with Meissa OT.

The therapy of patients in the home healthcare environment, requires training of each lay operator using the device, by the professional operator prior to the exercise. The lay operator must be trained in the safe and effective use of the device in therapy.

A lay operator may be considered a patient of the device, if they meet the patient requirements defined in chapter **6.1 Indications for use**. The training should cover all aspects, including how to respond to emergency

situations and safety hazards. **The professional operator should ensure that the knowledge and skills acquired by the lay operator will allow safe and effective operation of the device.**

Be aware that Meissa OT is designed for permanent installation if used in a home healthcare environment; therefore, it is essential to review the information provided in section **6.6 Use in a home healthcare environment**.

THERAPIST/ CLINICIAN - PROFESSIONAL OPERATOR - healthcare service providers of one of the following specialities: a physical therapist, an occupational therapist, a rehabilitation doctor, a neurologist, a nurse or nurse practitioner, an orthopedic doctor and other general practitioners.

Meissa OT is definitely a tool for you, to use in daily clinical practice (both in-patient and out), as well as to support your patients through telerehabilitation.

If you're a professional operator, you will be in charge of prescribing treatment procedures, including CPM, CAM, and in Meissa OT Ultra, the electrical stimulation parameters for your patients. Feel free to use this manual and the resources gathered here to expand your knowledge and find a quick guide on how to proceed with your patients.

We do expect professional operators to have graduated with a higher education degree of at least bachelors and are adults (at least 18 years old).

Please make sure that you fully understand the contents of this User Manual and the principles of electromyography and electrical stimulation, before you start working with your patients with Meissa OT. If you have any doubts, especially the **7. Warnings and basic safety** chapter, feel free to reach out to **EGZO**Tech directly and we will do our best to help you.

6.3 Contraindications

When **not to use Meissa OT** (contraindications):

- Acute, pronounced, severe, or persistent pain symptoms, despite conventional pain therapy in the trained extremity, or pain caused or intensified by the training.
- Unable to adjust to the patient position or anatomy.
  Do not carry out training with the system if the adjustment to the patient is not possible, e.g. due to individual physiologic position of the patient, patient's anatomy, limb sizes or lengths, contractures or severe spasticity (joint is fixed/rigid), or warped joint surfaces of the trained extremity.
- Severe joint rigidity, spasticity or extremely limited range of motion that can be negatively impacted by low-level passive movement training (risk of injury) (e.g. due to contractures, fixation within the joint, implants, spastic paralysis, arthrodesis etc.).
- Insufficient compliance from the patient, patients with severe psychotic, neurotic disorders or cognitive deficits impeding communication, uncooperative children, neuro-psychological conditions.
- Uncooperative or (self-) aggressive behavior, such as transitory psychotic syndrome.
- High-grade or severe ataxia.
- Fractures, osteosynthesis, advances osteoporosis, fracture risk, osseous instability, non-consolidated fractures, osteopenia, osteogenesis imperfecta, unstable vertebral column, pseudoarthrosis, osteomyelitis, considerably reduced bone density.
  Do not perform training in case of unstable or insufficiently consolidated fractures.
- Unstable vital functions (pulmonary or cardio-circulatory).
- Total or partial loss of sensitivity, e.g. due to lesions.
- Material intolerances, e.g. allergies to washing detergent, adhesive intolerances.
  There might be an allergic reaction to electrodes (Meissa OT Ultra only).
- Body or limb weight or dimensions exceeding technical specifications.
- Deep venous thrombosis.

- High-grade fever.
- Flaccid, spastic phase neurological lesions.
- Lesions in the acute phase of development.
- Hyperthermia.
- Irritation.
- Bleeding.
- Vascular lesions, vascular disorders of the trained limbs.
- Lesions in conjunctive tissue.
- Severe effusion.
- Joint instability.
- Osteomyelitis.
- Severe joint subluxation of the trained extremity.

Contraindications for Electrical stimulation only (Meissa OT Ultra only):

- Patients with cardiac demand pacemaker or any implanted defibrillator.
- No stimulation in the proximity of metal implants.
- Pregnancy (Electrical stimulation).
- Feverish or infectious diseases.
- Skin disorders subject to inflammation, as well as thrombosis or phlebitis.
- Body-worn electro-mechanical medical devices, i.e. insulin pump.
- Cardiac arrhythmia (do not use it on the chest).
- Serious arterial circulation problems in upper limbs.
- Abdominal or inguinal hernia.
- Patients with electronic life support equipment, such as respirators.
- Patients with electronic medical devices attached to the body, such as electrocardiographs.
- Patients with other electronic medical devices (device may cause erroneous operation of those devices).
- Placement of electrodes near the head / with current flowing through the carotid sinus or the chest with undiagnosed pain symptoms / disease.

Relative contraindications:

The treating physician or therapist evaluates the patient individually and must assess whether training with Meissa OT is suitable for the patient in case of:

- Apraxia.
- Epilepsy.
- Pacemakers and similar devices, other electrical stimulators, implants, including implanted medication pumps.
  Pacemakers can react differently to external influences. It is, therefore, important to be aware of relevant or possibly dangerous influential factors for the specific pacemaker model.
- Infections.
- Including septic tenosynovitis, until the infection is controlled.
- Untreated or uncontrolled infection.
- Joint problems, and degenerative bone diseases, including arthritis, arthrosis, bone cancer.
  Joint strain during training can cause pain and irritation in case of diminished load-bearing capacity.
- Neglect.
- Orthostatic circulation problems: increased risk of falling.
- Skin problems, swelling, skin ulcerations, open wounds, decubitus.

Before and after every training, check for previously existing wounds and wounds or pressure points caused by training, in particular in bodily areas that contact the device
- Shoulder-hand syndrome/subluxation, shoulder instability with uncontrolled shoulder displacement during training.
- Acute strain (musculotendinous unit) or sprain (non-contractile tissue).
- Soft tissue healing constraints (such as immediately after surgery).
- People with difficulties to understand should only use the device under supervision.
- Pregnancy.
- Acute inflammatory processes in the joints, unless on the order of a physician, inflammation, inflammatory diseases.
- Patients with (long-term) infusions.
- Severe postural instability.
- Patients who have been ordered to remain immobile.

This list is not meant to be exhaustive.

For patients with relative contraindications, it's possible to use Meissa OT with successful results, but having the parameters (maximal torque, maximal speed) set for the specific needs of that patient. Take extra caution when working with relative contraindications.

6.4 Facility responsibilities



Remember that Meissa OT is a device intended to help patients, but if used incorrectly, it may lead to injuries.

Home therapy can be performed if the patient was trained in using the device and is capable of performing training by himself. The device in home use can be used only in the pre-set configuration prepared by a professional user whether that's a physiotherapist or doctor for patient's therapy.

Be aware that Meissa OT is designed for permanent installation if used in a home healthcare environment; therefore, it is essential to review the information provided in section **6.6 Use in a home healthcare environment**.

Before working with a patient, the supervisor is required to familiarize the patient with the above indications and contraindications. The decision whether to use Meissa OT in a specific medical condition remains with the supervisor. All actions done by the supervisors and their consequences remains the facility. View the EULA (End User License Agreement) for details.

Engineers can operate the device during annual check-ups or service works – engineers are not allowed to work with patients.

EGZOTech Certified Trainers, engineers and service technicians can conduct device training on Meissa OT during product presentation.

For information about the nearest authorized representative or trainer, contact **EGZO**Tech.

6.5 Internet connection

The Internet connection allows you to fully utilize the potential of Meissa OT. The connection to the Internet is voluntary and largely depends on the safety policy of the health care facility. However, a permanent connection to the Internet allows you to keep the software updated.

Being disconnected from the Internet does not affect the basic functions and core operation of Meissa OT.



A reliable Internet connection is required to ensure the best user experience with Meissa OT. If your application does not work seamlessly, contact your product specialist.

6.6 Use in a home healthcare environment

Be aware that Meissa OT is designed to be permanently installed if it is used in the home healthcare environment, which means that the device is connected to the mains by a permanent connection that can only be disconnected using a tool by an authorized service personnel.



Connecting and disconnecting the AC cable by the user is not permitted.

The execution of permanent installation must be confirmed by completing the device connection protocol located in chapter 22. Meissa OT permanent installation protocol - home healthcare environment. Failure to complete this protocol will result in the forfeiture of the device warranty.



The installation, including a correct protective earth connection of Meissa OT, has to be carried out by qualified service personnel only!



The service personnel has to verify the integrity of the external protective earthing system.



The service personnel has to connect and verify that the protective earth terminal of the permanently installed medical electrical equipment is connected to the external protective earthing system.



Improper connection of the device in a home healthcare environment may result in electric shock, resulting in injury or death.

6.6.1 Guidelines for installing devices in a home environment

The precise requirements for an electrical installation in a home healthcare environment are shown below. Aligned with relevant standards that an authorized service personnel should follow to ensure compliance and safety.

1. Protective Earth (PE) Conductor

Requirement: A permanently installed protective earth conductor must be provided for all circuits that supply medical equipment. This conductor must be adequately sized to handle fault currents without excessive heating.

Standard Reference: IEC 60364 and BS 7671 specify the minimum cross-sectional area (CSA) for PE conductors, typically 2.5 mm^2 if mechanically protected or 4 mm^2 if unprotected. (BS 7671)

2. Residual Current Devices (RCDs)

Requirement: All circuits serving medical equipment in a home healthcare environment must include an RCD with a residual operating current not exceeding 30 mA. RCDs protect against potential electric shock by disconnecting the circuit within 40 milliseconds in the event of a fault.

Standard Reference: BS 7671 requires the use of RCDs for additional protection, especially in locations where individuals may be vulnerable. (BS 7671, Section 411)

3. Equipotential Bonding

Requirement: Equipotential bonding must connect all exposed conductive parts (e.g., metal frames of medical devices) and extraneous conductive parts (e.g., metal pipes) within the environment. This minimizes voltage differences, enhancing safety for patients and caregivers.

Standard Reference: Refer to IEC 60364-4-41 and BS 7671, which outline equipotential bonding requirements to prevent electric shock. (IEC 60364)

4. Socket-Outlets and Plugs

Requirement: Socket outlets must be installed with protective earth connections compatible with the power requirements of the medical equipment used. Ensure the outlet rating (voltage and current) is appropriate for the connected devices, typically 230V, 16A for standard equipment.

Standard Reference: IEC 60601-1-11 requires medical devices for home use to be connected to grounded outlets unless double-insulated. (IEC 60601-1-11)

5. Wiring Systems

Requirement: Use wiring systems with flame-retardant insulation to reduce fire hazards. Insulation must emit minimal smoke and toxic gasses in the event of a fire. Suitable cable types include LSZH (Low Smoke Zero Halogen) for these environments.

Standard Reference: BS 7211 specifies low-smoke, halogen-free wiring materials suited for healthcare environments, supporting fire safety regulations. (BS 7211)

6. Emergency Power Supply

Requirement: For critical medical equipment (e.g., ventilators, oxygen concentrators), an uninterruptible power supply (UPS) or standby generator must be available to maintain continuous operation during outages. Ensure backup power meets the device's rated power requirements.

Standard Reference: IEC 60364-7-710 provides guidelines on emergency power for medical locations, adapted here for critical home healthcare equipment. (IEC 60364-7-710)

7. Environmental Conditions and Protection Against External Factors

Requirement: The installation must withstand environmental factors, including temperature and moisture. Electrical outlets and equipment must have ingress protection (IP) ratings suitable for the area—e.g., IP44 in bathrooms or damp environments.

Standard Reference: IEC 60529 defines IP ratings, and IEC 60601-1-11 provides guidance on moisture resistance for home healthcare devices. (IEC 60529, IEC 60601-1-11)

8. Periodic Testing and Maintenance

Requirement: Conduct initial verification and periodic inspection/testing of all electrical installations and devices used in the healthcare environment to ensure ongoing compliance and operational safety.

Standard Reference: BS 7671 and IEC 60364 outline requirements for initial verification and regular testing intervals, especially in environments with vulnerable individuals. (BS 7671)

9. User Training and Documentation

Requirement: Provide clear operating instructions and user training for caregivers on safe equipment use and maintenance procedures. Maintain accessible documentation for all electrical installations and devices.

Standard Reference: IEC 60601-1-11 mandates clear user guidance and labeling for devices intended for home healthcare environments. (IEC 60601-1-11)

These requirements should be strictly followed by electrical engineers and verified during installation to ensure that home healthcare environments are safe, reliable, and compliant with applicable standards.

7. Warnings and basic safety



Meissa OT Ultra is an electrical medical device that incorporates a direct electrical connection with the patient's body with the intent of measuring electromyography and providing physiological currents through electrical stimulation as well as motorised movements of the patient's upper limb, such as CPM and CAM. As such, **Meissa OT Ultra can be dangerous if used incorrectly**. Please **read the safety information below and follow the guidelines provided in this manual**.

7.1 General safety consideration and precautions

Meissa OT has been created for specific physiotherapy exercises. **Do not use Meissa OT for any other purpose not included in this manual provided by EGZO**Tech.

Meissa OT produces results that are informative, not diagnostic. Qualified individuals must interpret these results.

Before starting to treat each patient or operate Meissa OT, you should at least read the information about the intended treatment, contraindications and safety measures.

The use of the device by a lay operator in a home healthcare environment requires prior consultation with a therapist/clinician - professional operator who will carry out a diagnosis, prepare an individualised therapeutic plan and provide training on a lay operator.

Meissa OT is intended to be used with the software running on the provided tablet. The tablet provided with Meissa OT has been chosen based on numerous parameters and has been configured for the best user experience. **Do not replace the provided tablet for any other device!** Using the software and/or Meissa OT with any other not intended device may lead to injuries.

Meissa OT cannot be operated on by a person whose motor skills are insufficient to fully operate the device, e.g. to stop it, disconnect cables or react to adverse situations. In such cases, professional care or assistance is necessary.

Keep caution while using Meissa OT in an event of changes in its performance. If any changes in Meissa OT's performance occur, contact **EGZO**Tech through one of the channels provided at the end of the user manual. Please refrain from using Meissa OT if you experience any performance changes.

Meissa OT has met the requirements of IEC 60601-1-2 for electromagnetic compatibility, including immunity, however **while running Meissa OT near high frequency / power medical devices, the safety manuals of those devices should be followed**. Incorrect use of other devices, and non-compliant devices may affect the parameters of Meissa OT.

Meissa OT is an automatic physiotherapy device. **Misconfiguring the training parameters**, especially electrostimulation parameters, range of motion, maximal applied torque and maximal speed **can lead to injuries!**

In the event that **Meissa OT does not behave as intended**, **press the emergency stop button** and notify your product specialist or our customer support immediately.

Emergency stop buttons do not switch off the power to Meissa OT entirely. In the event of a fire, water spill, or any other non-mechanical malfunction, step away from Meissa OT as soon as possible.

Any serious incident related to Meissa OT needs to be reported to **EGZO**Tech and the competent authority of the country in which the user and/or patient is based. Please inform us by sending a message to the following address safety@egzotech.com.

Use Meissa OT only with authorised accessories! This includes all the package contents listed in chapters **9. What will I find in the package?** and **11. Extensions**. Pay attention to their correct installation, use and maintenance.

Use only the AC cable supplied as specified in chapter 9.1.2 AC Power Cable. Do not plug in third-party sensors, electrodes or other accessories.

The usage of accessories not approved by **EGZO**Tech for use with the device is not permitted and may result in risk of injury, safety hazards or treatment failure. The use of such accessories may invalidate the terms of the warranty and cause other consequences not foreseeable by the manufacturer. Always confirm the use of electrodes not listed in this user manual with the manufacturer or the local distributor.

The use of improvised or non-approved limb fixing methods (e.g. elastic bandages), may delay emergency response and pose a risk to patient safety. If such methods are used, ensure they allow for quick release of the limb.

Meissa OT's measurement functions, including electromyography in Meissa OT Ultra, are susceptible to electromagnetic disturbances. As such, please be aware of other electromagnetic devices or installations that can affect measurements. Meissa OT meets the electromagnetic compatibility requirements, including immunity to electromagnetic disturbances, providing basic safety. If you encounter any signal artefacts or noise, discard the measurements and don't consider them diagnostically relevant.

Meissa OT Ultra is not intended to be used with needle electrodes.

Persistent use of the device in the presence of skin irritation may be injurious and may result in electrode burns.

Do not use Meissa OT outside of its operating environment requirements, including temperature or humidity, as specified in chapter **10.2 Technical Specifications** in this manual.

Do not use Meissa OT while sleeping.

Use of Meissa OT by a child is allowed only under the supervision of an adult.

The device should be kept out of the reach of children and pets.

Do not make any modifications to Meissa OT and the extensions. That includes removing the installed screws. Modifications to the device may affect the safety of the device and its compliance with safety and performance requirements.

The device and its accessories must be used in accordance with the conditions specified by the manufacturer in the user manual and other accompanying documents as well as in the form of markings on the devices, in particular on their labels.

When you are ready to finish working with Meissa OT, remember to release the extension and store it in the extension box.

Meissa OT shall only be used with the medical devices and medical device accessories specified in Section **9. What will I find in the package?** Meissa OT is not intended for simultaneous use or operation with any other medical devices or medical technologies. Use of the Meissa OT device in combination with other equipment or accessories may result in device malfunction, inaccurate therapy outcomes, or pose a risk to the safety of the patient, operator, or other persons. At the discretion of the professional user (therapist or healthcare personnel) responsible for the therapy, Meissa OT may be used with patients who have implants, pacemakers, or other medical devices, provided that an individual risk assessment has been performed by the professional user and that appropriate medical supervision is ensured throughout the therapy session.

Use of Meissa OT in combination with other products in a home environment is strictly prohibited.



Warning: Use of the device with visible damages is forbidden and can lead to injury. In case of any noticeable damages on the device, stop using the device and please contact the service.

7.2 Clinical safety

Warnings while using Meissa OT Ultra:

- No transcerebral applications,
- No stimulation in the vicinity of the carotid artery or carotid gland,
- No contralateral stimulation (i.e. positive and negative pole of the same channel on opposite sides of the body),
- Stimulation should not be applied transthoracically, as the introduction of electrical current into the heart may cause cardiac arrhythmias.

The patient should consult their clinician if there is any change in an existing condition or if any new condition develops.

Any serious incident related to Meissa OT needs to be reported to **EGZO**Tech and the competent authority in the country where the user and/or patient is based.

Using the device on patients with demand-type cardiac pacemakers may be hazardous.

Meissa OT produces results that are informative, not diagnostic. Qualified individuals must interpret these results.

Keep caution when using Meissa OT for patients with suspected or diagnosed heart problems.

Keep caution when using Meissa OT for patients with suspected or diagnosed epilepsy.

Keep caution when using Meissa OT for patients with body-worn electromechanical medical devices, such as insulin pumps, electronic medical devices attached to the body, and other medical devices, e.g. cochlear implants, electrical implants, or skeletal implants.

Keep caution when using Meissa OT with patients with serious arterial circulation problems in the upper limb.

Keep caution in the presence of the following:

- when there is a tendency to hemorrhage following acute trauma or fracture,
- following recent surgical procedures when muscle contraction may disrupt the healing process,
- over areas of the skin which lack normal sensation.

Patients should consult their physicians before using Meissa OT if they have any of the following:

- muscle atrophy,
- persistent pain,
- a history of trauma or a recent operation (less than 6 months prior),
- a need for muscle rehabilitation.

Do not use Meissa OT with patients if the user has reduced mental or physical capacity limiting the use of the device.

The use of Meissa OT should be immediately terminated upon any sign of treatment-related distress or discomfort.

The patient's position during therapy must be anatomically correct.

Electrodes should be used in accordance with their manuals or the instructions provided on the packaging, if they exist (Meissa OT Ultra).

Stimulation must not be applied in the presence of cancerous lesions in the treatment area or its immediate vicinity.

Setting the EMG activation threshold by the therapist or user either too high, preventing the patient from generating a sufficient signal to initiate the movement, or too low, leads to passive exercise without active patient control can lead to ineffective therapy, increased risk of patient discomfort or injury, potential frustration and adoption of compensatory movement strategies.

Pay attention to the patient's fatigue level during therapy. The long therapy sessions with a large number of repetitions without considering the patient's fatigue level can lead to reduced therapy effectiveness and side effects.

Pay attention to the correct adjustment of the spasticity detection threshold parameter, especially for spastic patients.

Patients with identified negative symptoms require evaluation of these symptoms and responses to them.

7.3 Electrical safety and electromagnetic compatibility

Meissa OT is running on specific electrical parameters. **Ensure that you have a compatible AC socket with the requirements specified** in chapter **10.2 Technical Specifications**.

In an event that **Meissa OT doesn't behave in an intended manner, turn the power switch off** and notify your product specialist or our customer support immediately.

WARNING: To avoid risk of electric shock, this equipment must only be connected to a supply mains with protective earth.

Meissa OT is an electrical device with IP21 liquid ingress and solid particle protection. If possible, protect Meissa OT from contact with liquids and/or solid particles.

Avoid stretching, riding over, tying up, or any activity that could damage the AC cable, EMG/EMS cables or tablet's holder. Do not pull on the AC cable (and EMG/EMS cable). Hold the cables by the plug when connecting or disconnecting.

To unplug the device from the power supply pull the plug (not the cord) or use the installation disconnector. Never pull cables connected to the device or the installation. If you want to move a permanently installed device, pay attention to move it only as far as the AC cable allows you.

Do not turn OFF the mains power of the device during therapy (except in an emergency).

Do not transport Meissa OT while it is connected to the power supply.

While replacing external AC fuses, follow the electrical requirements specified in chapter **10.2 Technical Specifications**.

Use only IEC C13 AC cables that have dual isolation and comply with the electrical requirements in the technical specification.

Meissa OT is electrically safe, even in the event of a single subsystem failure. Nevertheless, if you witness any problems regarding cables, chassis, or any safety elements in spite of its detection in the software, take extra caution and contact your product specialist.

Meissa OT has BF type applied parts (elements that are intended to get in contact with a patient). Applied parts are used to transfer mechanical energy to the patient (make the patient limbs move), and to transfer electrical energy from and to the patient (Meissa OT Ultra only) Those parts have extended electrical safety parameters and are labeled according to the symbols table in chapter **8.4 Symbols**.

Do not connect leads or electrodes to other objects.

Do not use Meissa OT Ultra if you are connected to a high-frequency surgical equipment, as this could cause skin irritations or burns under the electrodes.

Meissa OT has met the requirements of IEC 60601-1-2 for electromagnetic compatibility, including immunity, however **while running Meissa OT near high frequency / power medical devices, the safety manuals of those devices should be followed**. Incorrect use of other devices, and non-compliant devices may affect the parameters of Meissa OT.

Simultaneous connection of the patient to a high-frequency surgical device and to an electromyograph or to a device for recording burst biopotentials can cause burns at the site of application of the electrical stimulator electrodes or electrodes of the input part for biopotentials, as well as possible damage to the electrical stimulator or biological amplifiers (Meissa OT Ultra only).

Do not use Meissa OT Ultra unit within 1.5 meters of shortwave or microwave devices, as this could alter the output generated by the stimulator. If you have any doubts when using the stimulator in close proximity to another medical device, please contact the device manufacturer or your doctor.

Meissa OT complies with the requirements of IEC 60601-1-2 (EMC Collateral Standard) including the E-field susceptibility requirements at a level of 10 V/m, at frequencies from 80 MHz to 2.7 GHz. However, even at this level of device immunity, certain transmitting devices (mobile phones, two-way radios, cordless phones, paging transmitters, RFID devices, etc.) emit radio frequencies that could interrupt Meissa OT operation if operated in a range too close to Meissa OT. Practitioners should be aware of possible radio frequency interference if portable devices are operated in close proximity to Meissa OT.

Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of Meissa OT, including cables. Otherwise, degradation of the performance of this equipment could result.



Warning: Keep RFID readers at least 30 cm away from the device.



Warning: Operation in close proximity to a shortwave or microwave therapy equipment may produce instability in the applied part.

Keep caution to avoid accidental contacts between Meissa OT Ultra's patient lead wires and/or electrodes with other equipment with conductive parts, including parts connected to the ground.

If you witness any wear and tear problems or damage regarding cables, chassis, or any safety elements, take extra caution and contact **EGZO**Tech.

The use of accessories, transducers and cables other than those specified or provided by **EGZO**Tech for this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Avoid using this equipment adjacent to or stacked with other equipment, as this could result in improper operation. If such use is necessary, this equipment and the other equipment should be monitored to ensure they are operating normally.

The connection ports of Meissa OT's Head are intended for specific accessories mentioned in this user manual. Do not connect any other devices to those ports.

Meissa OT has four extension connector pins located on the front of the Head. Those connectors are used to power the extension. While working with Meissa OT, patient should not touch these connectors, either directly or indirectly through you (the patient should not touch the supervisor while they are touching these connectors).

The electrostimulation treatment must be stopped before disconnecting the electrodes (Meissa OT Ultra only).

7.4 Electrical stimulation safety, including TENS (Meissa OT Ultra only)

Electrical stimulation should **only be used after training from a healthcare professional**. Always consult your physician before using electrical stimulation, to choose the right output parameters and program for you. Improper selection of electrostimulation parameters can result in patient ailments due to excessive electrostimulation or a lack of therapeutic effects due to insufficient electrostimulation.

Never touch electrodes directly during electrical stimulation. In case of distress or unexpected operations of Meissa OT Ultra, press the emergency button.

Always check the impedance, the distance between the electrodes, and their wear and tear between uses. Using worn or torn electrodes may cause severe burns.

Always apply both poles (+) and (-) of each channel to the same muscle to be electrostimulated. Application of (+) and (-) electrostimulation channels on different muscles may result in lack of therapeutic effect due to improper stimulation, risk of burns on the patient, potential risk of electric shock.

Do not use electrical stimulation while wearing clothes lined with, made with or containing conductive (especially metal) materials. Do not apply stimulation near metal elements. Remove jewelry, body piercings, belt buckles or any other removable metallic product or device in the area of stimulation. Metals on the body and within worn clothes can conduct electricity during electrical stimulation, causing severe burns. Metal can also impact electromyography measurements.

The long-term effects of chronic electrical stimulation are unknown.

Stimulation should not be applied over the carotid sinus nerves, particularly in patients with a known sensitivity to the carotid sinus reflex.

Stimulation should not be applied over the neck or mouth. Severe spasm of the laryngeal and pharyngeal muscles may occur, and the contractions may be strong enough to close the airway or cause difficulty in breathing.

Stimulation should not be applied transthoracically, as the introduction of electrical current into the heart may cause cardiac arrhythmias.

Stimulation should not be applied transcerebrally.

Stimulation should not be applied over swollen, infected, or inflamed areas or skin eruptions, e.g., phlebitis, thrombophlebitis, varicose veins, etc.

Stimulation should not be applied over or in proximity to cancerous lesions.

Stimulation should not be applied across or through the head, directly on the eyes, covering the mouth, on the front of the neck (especially the carotid sinus), or from electrodes placed on the chest and the upper back or crossing over the heart.

Stimulation should not be applied in proximity of abdominal or inguinal hernia because the great tension in the abdomen and pelvic floor may worsen this condition.

Stimulation should not be applied in proximity of the abdomen and back for the patients with intestinal clamps.

During a stimulation session, do not disconnect electrodes when stimulation is running. Stop the stimulation first.

For output exceeding 10 mA or 10 V, please ensure to use electrodes that meet those output requirements.

The safety of TENS devices or powered muscle stimulators for use during pregnancy or delivery has not been established.

TENS is a symptomatic treatment and as such may suppress the sensation of pain, which would otherwise serve as a protective mechanism on the outcome of a clinical process.

Electrode placement and stimulation settings should be based on the guidance of the prescribing medical practitioner.

Special attention from the operator is required when current density exceeds 2 mA/cm^2, as a hazard could exist if excessive current densities are present. Electrodes of inadequate size or unsuitable application could provoke skin reactions or burns.

Powered muscle stimulators should be used only with the leads and electrodes recommended by the manufacturer.

Portable powered muscle stimulators should not be used while driving, operating machinery, or during any activity in which involuntary muscle contractions may put the user at undue risk of injury.

Skin irritation and burns beneath the electrodes have been reported with the use of powered muscle stimulators. If skin irritation occurs, discontinue use and consult your physician.

If the stimulation levels are uncomfortable, reduce the stimulation intensity to a comfortable level and contact your physician if problems persist.

TENS is not effective for pain of central origin, as compared to pain of peripheral origin.

TENS is of no known curative value.

The treatment outcome will be influenced by the patient's psychological state and use of drugs.

TENS should be used only under the medical supervision of a physician or under the supervision of a qualified medical practitioner to whom the patient is referred by a physician.

Do not use electrical stimulation with cardiac demand pacemakers, implanted defibrillators, or other implanted electronic devices unless specialist medical opinion has been obtained first.

While using electrical stimulation electrodes, ensure that the impedance displayed in the software is correct. The adhesive properties of electrodes do not guarantee good conductivity.

Cutting or modifying electrostimulation electrodes can lead to ineffective stimulation, potential damage to the electrodes, causing them to malfunction. There may be an increased risk of skin irritation or burns due to improper contact or electrical conductivity. Furthermore, this may reduce the safety of the therapy, potentially leading to patient injury or discomfort.

Use only electrodes authorized by **EGZO**Tech, as described in chapter **9.4 Electrodes for electrostimulation**. **Using electrodes that are the wrong size or not suited for the application could lead to skin reactions or burns**. Electrode properties, such as dimensions, conductivity, impedance, and connector types, can greatly impact safety. **Never use ECG/EMG electrodes for electrical stimulation.**

Electrodes should be used in accordance with their user manuals or the instructions provided on the packaging (if available).

During electrical stimulation (Meissa OT Ultra only), ensure that neither the patient nor the therapist touches the Arm Support. Only the patient's upper limb should rest on the cushion (either small or large) and be secured with a strap.

7.5 Mechanical safety

Meissa OT has trapping zones between the extension and head and/or platform, and between parts of foldable Arm Support.

Do not place any body parts or other objects in any of these trapping zones while Meissa OT is moving. Placing objects in the trapping zones during normal operation may cause injuries.

The device must be fully visible at all times during use. Never cover the device (e.g. with bed linen or any other material) during operation.

Before use, always check Meissa OT and accessories (inc. extensions) for mechanical damages. Do not use Meissa OT or any accessories (inc. extensions), when a damage was noticed.

Do not make any mechanical modifications to Meissa OT and accessories (inc. extensions), That includes removing the installed screws.

In the rare event of an uncontrolled, unintended movement of Meissa OT, press the emergency stop first, and then proceed with unstrapping your patient from the extension (if needed).

While using Meissa OT, avoid wet, slippery, or uneven surfaces. Try to avoid these during transportation or mounting whenever possible.

Do not step, sit, or stand on any part of Meissa OT or its accessories (inc. extensions). Do not place any unintended objects on Meissa OT.

Do not use Meissa OT in a dangerous environment (including explosion risk, gas risk, etc.).

Please report all damage, malfunctions, or unusual behaviour to your product specialist.

Always use cables with the minimum number of channels necessary for the training to limit unnecessary risk.

Keep small children away and take care not to get entangled in the patient lead wires. Strangulation and asphyxiation are possible! Consider using shorter cables (available on request).

Use Meissa OT only on firm, flat, level surfaces.

Simultaneous use of two devices for exercising both upper limbs is not permitted.

Before therapy, patients need to be instructed on the location of the emergency button and how to stop the device in case of discomfort, pain, irritation or other dangers. Patients who are unable to use the emergency button during therapy should not be left without supervision of the operator.

Before starting therapy with a patient, run several cycles without the patient to test the full range of the device.

Always plug the least amount of channels, as needed for the training, to limit unnecessary risk.

Keep small children away and keep caution not to inhale or swallow small parts due to the choking hazard.

Meissa OT uses its weight and a mounting system for stability. **Follow the maximum joint weight and maximum torque stated in the technical specification** to avoid instability and toppling over.

Before starting training, ensure that the platform and all device axes are locked in place.

Always ensure that the table clamps are correctly installed. Improperly mounted clamps pose a risk of accidents and potential injury to the patient or therapist.

Before use, ensure that the cushion, clamp, and Arm Support are correctly mounted, with the Arm Support securely attached to the clamp and the clamp firmly fastened to the tabletop. Do not use the accessory if any part is missing. During adjustment procedures, there is a risk of hand injury. Pay special attention to the limbs of both the operator and the patient while setting up the Arm Support.

The maximum safe working load for the Arm Support is 5 kg in its fully-extended position and 10 kg in half-extended position. However, be aware that applied load may cause damage to the tabletop, on which the Arm Support is mounted. Therefore, always pay attention to the Arm Support and the tabletop during use to prevent potential damage and injury.

Do not adjust the height of the Electric Table during exercises or when the patient is secured to Meissa OT or the Arm Support. The risk of discomfort or injury to the patient.

Ensure that there are no obstacles near the table that could hinder or prevent its adjustment, as this could pose a risk of damaging the table or the obstacles.

A tabletop with a thickness of less than 18 mm that is not supported from below by a steel frame may break during the use of Meissa OT, posing a risk to both the patient and the operator. It is recommended to use tabletops with a thickness greater than 18 mm.

Before transportation, make sure that the platform's mounting system is unlocked.

If you need to transport Meissa OT, use the provided transport box, for internal transport it is permissible to move unboxed in the transport position within one building.

During transportation, avoid collisions with other objects.

Beware of the risk of dropping the device during transportation. **In the event of dropping, the device must not be used until it has been repaired, fully functionally tested and safety tested** by an authorised manufacturer's service personnel. Please mind that the underestimation of the device's weight, details in **10.2 Technical Specifications** may lead to handling difficulty.

7.6 Multiple use precautions and consumables

Meissa OT has been tested for reliability during multiple uses and cleaning with the disinfection products described in chapter **19. Cleaning**. The use of different cleaning products can yield varying results and may lead to contamination, surface deterioration, loss of biocompatibility and malfunction.

The device is neither intended to be sterilized nor supplied sterile.

Caution should be used for the disposal of Meissa OT. Meissa OT should not be thrown out, or improperly disposed of due to electronic components. To avoid biological contamination of the environment, remember to clean and disinfect the device before disposal. Consult your product specialist on how to act best to utilize Meissa OT that won't negatively impact the environment.

Surface electromyography electrodes are designed for single-use. Using the same electrodes multiple times will lead to signal degradation and possible misuse and incorrect evaluation (Meissa OT Ultra only).

Meissa OT accessories and the device itself will experience normal wear and tear over time. Performance degradation is possible over time, especially in electrical connections between the cables and electrodes, as well as between snaps and electrical stimulation electrodes themselves.

For bioelectric programs (like electromyography in Meissa OT Ultra only), we recommend using single-use electrodes. **Remember to use single-use electrodes only once**. If you decide to use different electrodes, always consult your product specialist.

Remember to clean the multiple-use electrodes as intended by the manufacturer.

Electrical stimulation electrodes are intended for use by one person only and may only be reused in accordance with their manufacturer's instructions on the packaging/label or in the accompanying documentation. Note: The lifetime of the electrode varies depending on skin conditions, skin preparation, type of stimulation, storage, and climate (Meissa OT Ultra only).

Meissa OT is a specialised electrical device and contains dangerous voltages inside, **therefore, maintenance is limited to authorised EGZO**Tech **personnel only**. If a malfunction occurs, call your product specialist or our

customer support immediately. **EGZO**Tech provides the necessary technical information to all maintenance personnel.

Meissa OT is intended for constant use, however, it is equipped with temperature sensors and early failure detection algorithms. In the rare event that Meissa OT stops the current operation, it will display a notification about current system status (e.g. malfunction, etc.). There is no danger in this case, but Meissa OT will cease all operations until the issue has been resolved, either automatically or by a product specialist or customer support.

Before working with patients, Meissa OT must perform a diagnostic procedure to ensure maximum safety. You will not be able to run any training programs until the results from the diagnostic tests will comply with intended safety standards. Follow the software instructions after the quick setup guide to complete these steps.

7.7 Biological safety

Never use Meissa OT **with compromised or wounded skin**.

Meissa OT is intended for surface (intact skin) contact only. **Avoid contact with mucosal membranes, breached or compromised surfaces**, or in any case, inside your body.

Meissa OT has been analysed for biocompatibility, including cytotoxicity, sensitization, irritation, and intracutaneous reactivity. However, **if you or your patient experience an allergic reaction, irritation, or signs of toxicity - whether from Meissa OT or any other source - cease all training** until the underlying cause has been addressed.

Meissa OT's materials have been tested with the disinfection products described in chapter **19. Cleaning**. The use of different, especially unintended disinfection, products can lead to contamination, surface deterioration, loss of biocompatibility, and malfunction.

Some patients may experience skin irritation or hypersensitivity due to the electrical stimulation or electrical conductive medium. This irritation can usually be reduced by using an alternate conductive medium or alternate electrode placement (Meissa OT Ultra only).

Clean and disinfect Meissa OT after every patient to avoid transmission of infectious skin diseases.

The user or the medical service provider must contact its local authorities to determine the proper method of disposal of potentially biohazardous materials, including but not limited to: surface electrodes and other Meissa OT accessories.

7.8 Environmental safety

Do not perform service, maintenance, or modifications on Meissa OT yourself! Use only service providers authorized by **EGZO**Tech. Actions carried out by unauthorised personnel may result in improper repair or damage to the device and a risk of reduced safety for the user and the device.

Do not attach the table mounting clamp and Meissa OT to the metal table! After installing Meissa OT device, ensure that **no part of the device or its accessories comes into contact with the metal components** of the table, cabinet, or any other object on which it has been installed before use - there is a risk of electrical shock or burns.

Always use and store Meissa OT, the accessories and electrodes according to their storage instructions. Please consult the accompanying documents for electrode storage instructions.

Do not use Meissa OT in an oxygen-rich atmosphere.

Do not use Meissa OT in a dangerous environment (includes explosion risk, gas risk, etc.).

Meissa OT is intended for use in a moisture-free environment. Keep it away from water, including that generated by other devices, e.g. kettles, nebulisers, showers etc.

Meissa OT is intended to be used in the operating temperature and humidity specified in chapter **10.2 Technical Specifications**.

Meissa OT is intended to be used in a home environment, a home healthcare environment (e.g. retirement homes), and a healthcare environment (e.g. hospital, clinic). Be aware that Meissa OT is designed for permanent installation if used in a home healthcare environment; therefore, it is essential to review the information provided in section **6.6 Use in a home healthcare environment**.

Meissa OT should be used in well-lit rooms.

Meissa OT is intended for indoor use only.

Dust, water, lint or other pollutants can interfere with electronics, especially if they are located near the cable connectors. Please clean Meissa OT periodically, according to chapter **19. Cleaning**.

Due to the device's sensitivity and risk of damage during improper handling, please keep it away from children, pets and pests.

Meissa OT Ingress Protection code (IP) is specified in the chapter **10.2 Technical Specifications**. The rating is IP21, therefore:

- IP2X for solid particle protection of objects larger than 12.5 mm (0.49 in). This means that the enclosure provides protection against hazardous parts, especially electrical conductors, and the ingress of solid foreign objects of the mentioned size.
- IPX1 for liquid ingress protection of dripping water. This means that the enclosure provides protection against harmful ingress of water to the extent of vertically dripping water.

Do not immerse Meissa OT in water or any other liquid substance, including water vapour.

7.9 Software safety and cybersecurity

Do not use other applications while using Meissa OT app, as this can disturb normal operations.

Meissa OT is delivered by **EGZO**Tech with a preconfigured third-party ICT device (tablet) with restricted access. Do not install any unapproved applications. Untested software can interfere with the normal operations of Meissa OT.

Software updates include safety enhancements, allow Meissa OT to update as notifications arrive.

A reliable Internet connection is required to ensure the best user experience with Meissa OT. If your application does not work seamlessly, contact your product specialist.

7.10 Lifetime

Meissa OT, due to its moving **mechanical parts, will experience wear and tear**. Because some safety features are implemented using these mechanical parts, periodic maintenance is required based on your Meissa OT usage. With the implementation of two methods of patient protection for mechanical dangers, maintenance of Meissa OT can be performed after a single fault has occurred. Official maintenance personnel approved by **EGZO**Tech or its partners can conduct **periodic maintenance to ensure continuous stability and reliability of the device, preventing single fault conditions**. If your Meissa OT has a stable, unrestricted Internet connection available at all times, your usage will be monitored by **EGZO**Tech and its partners, and necessary maintenance will be proposed ahead of time to limit the downtime of your devices.

Periodic inspections should be performed in accordance with the terms of the sales and warranty agreements.

7.11 Annual maintenance



To ensure the continued safety and reliable operation of Meissa OT, **annual tune-up maintenance is required**.

Regular servicing is essential to meet medical device safety standards, and skipping the annual maintenance may compromise device performance or safety.

We strongly recommend that you do not miss the scheduled tune-up. In the event of unforeseen issues, please contact your provider immediately.

Please note that **EGZO**Tech cannot be held liable for any consequences resulting from the omission of the required annual maintenance.

The device should be cleaned and disinfected before submission for service or repair to prevent cross-contamination and health risks to service personnel.

7.12 Risk and benefits

As a medical device, Meissa OT was developed for therapeutic application of upper limbs. Meissa OT is intended for motor rehabilitation of upper limbs. You can find a complete list of indications in chapter **6.1 Indications for use**.

Meissa OT Pro has safety features to provide complex treatment based CPM and CAM motorized movements of upper limb muscles. Meissa OT Ultra has safety features to provide complex treatment based on electromyography biofeedback and electrical stimulation used in CPM and CAM motorized movements of upper limb muscles. The positive treatment results were confirmed and a concept of the device is well described in literature, based on the clinical trials. Relying on the clinical literature research, clinical evaluation and the similar devices introduced on the market the effectiveness of the treatment concept is confirmed.

Available information for similar devices and risk analysis conducted by manufacturer indicated that likelihood and severity of risk for Meissa OT is low. Meissa OT fulfills safety requirements included in standards.

Based on clinical evaluation, the benefits of using Meissa OT device in both therapeutic and evaluation scope, along with the implemented measures to limit potential risks, indicate that the benefits significantly outweigh the potential risks.

The patients should consult their clinician if there is any change in an existing condition or if any new condition develops.

Any serious incident related to Meissa OT has to be reported to **EGZO**Tech and the competent authority of the country where the user and/or patient is located.

Meissa OT produces results that are informative, not diagnostic. Qualified individuals must interpret the results.

The use of Meissa OT should be immediately terminated upon any sign of treatment-related distress or discomfort.

The manufacturer provides appropriate warnings and labeling which limits the possible risk.

8. How to work safely with Meissa OT?

8.1 Why this user manual is so important

Remember that Meissa OT is an automatic physiotherapy robot. This means it can function as a standalone exerciser for your patients. However, **misconfiguring the training parameters** - especially electrostimulation parameters, range of motion, maximal applied force, and maximal speed - **can cause injuries!**


Do not start using Meissa OT before being familiar with this user manual.

8.2 Labelling

On the back of the device, you will find the main label of Meissa OT. This label contains information about the specific unit of Meissa OT that you own. Additionally, Meissa OT uses safety symbols on the device itself, as well as within the software application and on packaging of accessories. Below are Meissa OT's labels.

Due to the ongoing transitional period, the device may be supplied with one of the labeling versions listed below. The specific label applied depends on the device model and production batch.


Meissa OT Ultra EU Label:

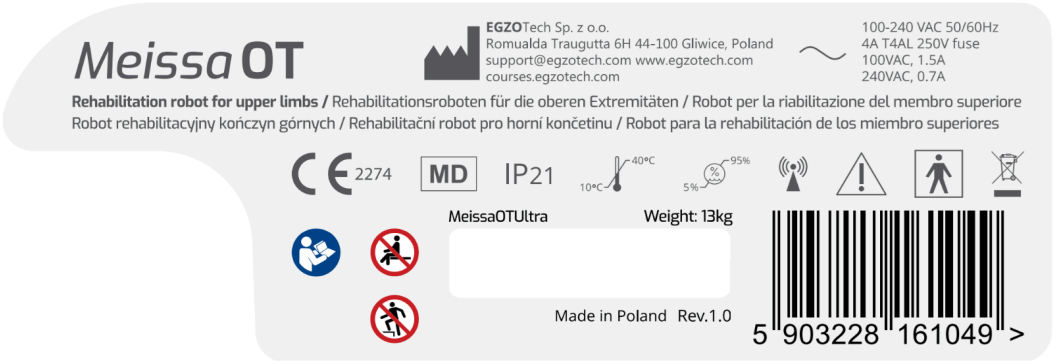

Meissa OT Pro EU Label:




Meissa OT universal Label:

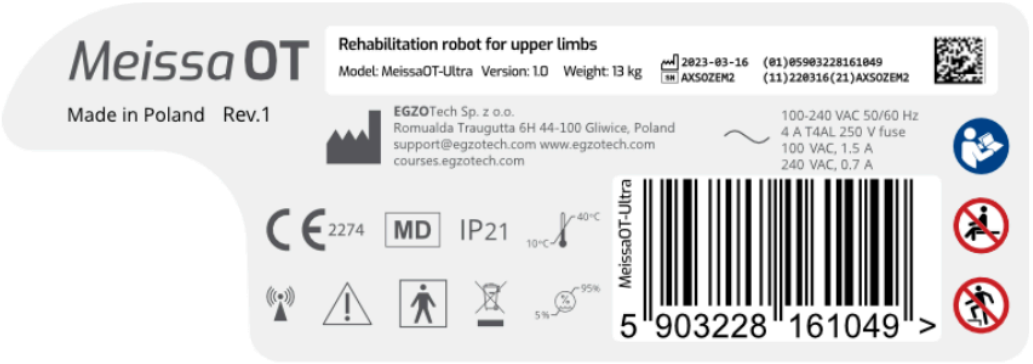

8.3 Software Version Identification

The current version of the software installed on the device is displayed on the login screen in the highlighted area.

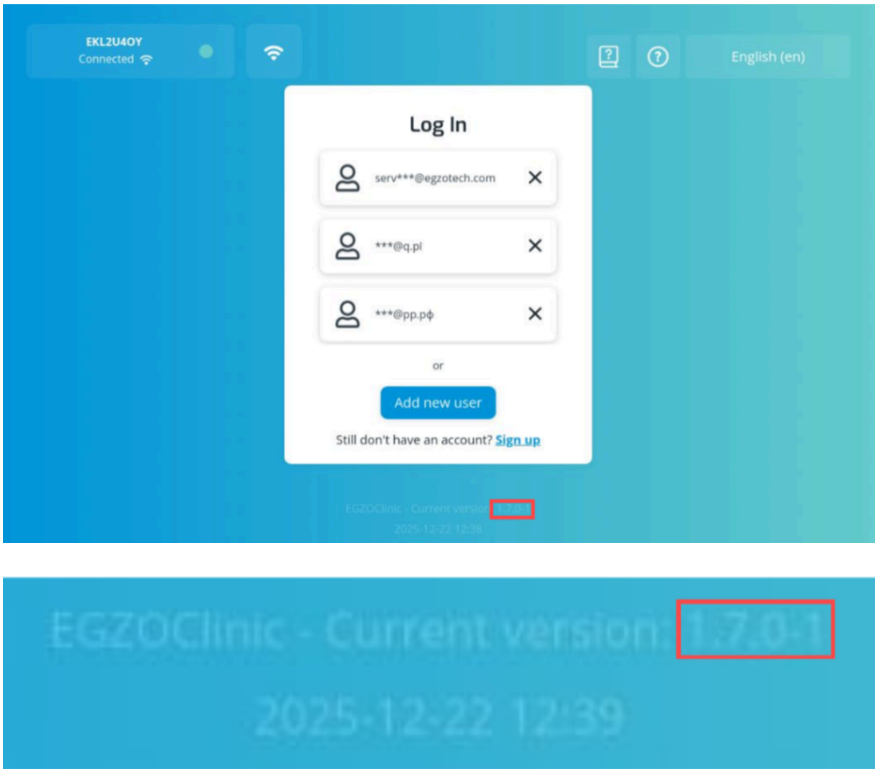

8.4 Symbols

Meissa OT uses safety symbols on the device itself, as well as within the software application and on packages with accessories. Below is an explanation of all the symbols you may encounter while using Meissa OT:

Symbol	What it means	Symbol	What it means
	Manufacturer	MD	Medical Device

Symbol	What it means	Symbol	What it means
 YYYY-MM-DD	Manufacturing Date		Serial Number
 YYYY-MM-DD	Manufacturing Date with Country of Origin (Poland)		The CE marking indicates that a product complies with applicable European Union regulations. No. 2274 is the number of the Notified Body
	FCC mark		Indicates the need for the user to consult the instructions for use
Made in Poland	Indicates Poland as the Country of Origin		Caution is necessary when operating the device or control near the location of the symbol, as the current situation may require operator awareness or action to avoid undesirable consequences
IP21	Ingress Protection (IP code)		The product should not be disposed of as unsorted waste but must be sent to separate collection facilities for recovery and recycling
	Main Power Switch	 courses.egzotech.com	Indicates the need for the user to consult the instructions for use
100-240 VAC 50/60 Hz 4A T4AL 250 V fuse 100 VAC, 1.5 A 240 VAC, 0.7 A	Indicates range of permissible power supply parameters and type of fuse used in the device		The device generates radio frequency energy during operation
	Applied part type BF, used for electrical connections to and from the patient. This part is		Emergency Button

Symbol	What it means	Symbol	What it means
	isolated from all other parts of the device		
	Indicates the temperature limits to which the medical device can be safely exposed		Indicates the humidity limits to which the medical device can be safely exposed
	No sitting on the device		Not stepping on the device
	Medical device packaging and contents should be kept dry		This way up
	Indicates a medical device that can be broken or damaged if not handled carefully		Do not stack
	Do not roll		Warning; Crushing of hands - To warn of a closing motion of mechanical parts of equipment
	General warning sign - To signify a general warning		Warning; Crushing - To warn of moving mechanical parts
 XXXXXX	Model number - indicates the model number		Maximum device weight - indicated maximum device weight without accessories

8.5 Accessories symbols

Symbol	What it means	Symbol	What it means
	Indicates the manufacturer's catalog number so that the medical devices can be identified		Indicates that a medical device should not be used if the package has been damaged or opened, and that the users should consult the instruction for use for additional information
	Indicates the date after which the medical device is not to be used		Indicates a medical device that is intended for one single use only
	Silver/silver chloride sensor		Latex free
	Indicates a medical device that requires protection from light sources		PVC free
	Indicates the manufacturer's batch code so that the batch or lot can be identified		Bulk packaging quantity

9. What will I find in the package?

Depending on your order and configuration, you may find the following products associated with Meissa OT included in the package.

For any aspects related to accessories that are not specifically addressed in this section, the general guidelines and procedures outlined in this manual should be followed, particularly regarding cleaning, disinfection, and disposal.

9.1 Meissa OT

What does it look like?	Description
	Meissa OT Rehabilitation robot for upper limbs 1 pc.

9.1.1 Extensions

9.1.1.1 Extension for elementary movement

Extension for elementary movements that can be used for exercises listed below:

- Forearm pronation and supination,
- Radial and ulnar wrist deviation,
- Wrist flexion and extension.



9.1.1.2 Occupational therapy extensions

What does it look like?	Description	What does it look like?	Description
	Ball extension Code: MO-Ext-01 1 pc.		Pinch meter extension - large Code: MO-Ext-03 1 pc.
	Handle extension Code: MO-Ext-04 1 pc.		Disc extension - small Code: MO-Ext-08 1 pc.
	Screwdriver extension – small Code: MO-Ext-11 1 pc.		Mixer extension Code: MO-Ext-12 1 pc.

9.1.2 AC Power Cable

The cable included with the device may vary depending on the order specifications and the environment in which the device will be used.

What does it look like?	Description
	**AC Power Cord** 250 V / 10 A / H05VV-F Class 1 protection acc. to IEC 61140 Device plug: C13 acc. to IEC 60320-1 Socket plug: CEE 7/7 (E & F compatible) standard * Length 5 m - 1 pc. **For professional use only**

	**AC Power Supply Cord for home healthcare environment** 250 V / 10 A / H05VV-F Class 1 protection acc. to IEC 61140 Device plug: **C13 with LOCK** acc. to IEC 60320-1 VERIFIED PERMANENT CONNECTION to POWER NETWORK is required Length 5 m - 1 pc. **For home healthcare environment dedicated cable.** Be aware that Meissa OT is designed for permanent installation if used in a home healthcare environment; therefore, it is essential to review the information provided in section **6.6 Use in a home healthcare environment**. If you want to move a permanently installed device, pay attention to move it only as far as the AC cable allows you.

* Other socket plugs are available upon request. Please contact **EGZO**Tech Sp. z o.o. or your local distributor.

9.1.3 Table mounting clamp

The table mounting clamp is designed to prevent Meissa OT from sliding on the table during patient use.

The table mounting clamp can be attached to surfaces with a **thickness ranging from 10 to 40 mm**.



Do not attach the table mounting clamp to the metal table!


After installing Meissa OT device, ensure that **no part of the device or its accessories comes into contact with the metal components** of the table, cabinet, or any other object on which it has been installed before use - there is a risk of electrical shock or burns.

9.2 EMG/EMS cable - 1 pc. (Meissa OT Ultra only)

4 channels EMG/EMS cable - 1 pc.

- Consists of 4 channels for EMG/EMS + 1 reference channel for EMG
- All channel cables and reference cable are combined into one connector (MDR connector)
- Each channel cable has 2 separate wires coming out of the splitter
- Lengths of channel cables:
  - Channel 1: 150 cm
  - Channel 2: 150 cm
  - Channel 3: 120 cm
  - Channel 4: 120 cm

- Reference (REF) cable: 120 cm

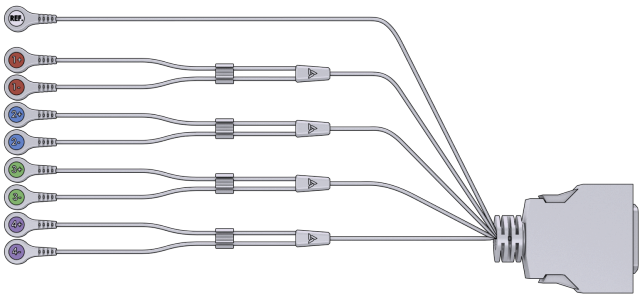

To properly connect the MDR cable with the device, remember:

- Check the MDR connector orientation - make sure it is properly aligned with the socket, it only fits one way.
- Insert the connector straight and evenly into the socket.
- The connector should slide in with slight resistance and “click” or stop firmly when fully inserted. If you feel strong resistance - stop and recheck the alignment.
- The side buttons of the MDR connector should bounce when the plug is correctly inserted into the socket.
- Verify the connection. Make sure the device recognizes the cable.

Pay attention to the cable routing of the EMG/EMS cable, positioning and routing in a way that protects the cables from mechanical and electrical damage. Ensure that the cables are not entangled with the head, applied parts or tablet holder, that there is no risk of the cables being accidentally pulled by the patient's limb or snagged on other components. Do not stress the cables, as this may result in damage to the cables or disconnection from the electrodes.

To properly disconnect the MDR cable from the device, remember:


- Hold the connector housing firmly — never pull on the cable itself.
- Press both side buttons simultaneously to unlock the connector from the port. These buttons are designed to gently release the plug from the socket without damaging the pins.
- While holding the buttons, pull the connector straight out, slowly and evenly. Avoid pulling at an angle or twisting.
- Once removed, store the cable properly to avoid bending or straining the pins.

Avoid the following:

- Do not pull on the wires — this can damage internal connections.
- Do not force the connector out without pressing the release buttons – this may damage both the connector and the device.
- Do not use tools like screwdrivers to pry it out — this may damage both the cable and the device port.
- Do not remove it at an angle — this can bend or break the pins.

9.3 Electrodes for surface electromyography (Meissa OT Ultra only)

The table below presents the electrodes that are approved and safe for use with surface electromyography using Meissa OT Ultra. However the type and quantity of electrodes provided with the device depend on the order specifications and may vary.

What does it look like?	Description
	ECG surface electrode **EGZOTech EE S5540 FWG** Area intended to contact the surface of the skin: 22 cm^2 55 x 40 mm 50 pcs./case
	ECG surface electrode **EGZOTech EE S5540 FWG1** Area intended to contact the surface of the skin: 15.4 cm^2 44 x 35 mm 50 pcs./case

Meissa OT Ultra is compliant with any surface ECG/EMG electrodes that meet IEC 60601-1 requirements. The device is designed for use with snap electrodes; using other types of electrodes requires an adapter.

Before use, always check and follow the information provided by the electrode manufacturer.


Always **confirm the use of electrodes** not listed above **with the manufacturer or the local distributor**. The use of electrodes not listed in the table above or not confirmed by the manufacturer or local distributor may result in device malfunction, failure to operate, or **pose a burn risk to the patient**.



The **size of the electrodes** should be selected **appropriately for the area** of application.

The choice of electrode is determined by the professional user, who should have the necessary knowledge to specify this. The user using the device in a home healthcare environment (lay operator) should only use the electrodes indicated by the therapist.

9.4 Electrodes for electrostimulation (Meissa OT Ultra only)

The table below presents the electrodes that are approved and safe for use with electrostimulation using Meissa OT Ultra. However the type and quantity of electrodes provided with the device depend on the order specifications and may vary.

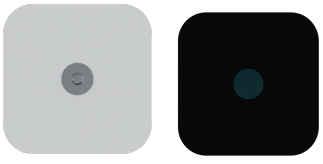What does it look like?	Description
	Small electrical stimulation electrode **UltraStim Snap SN2020** Area intended to contact the surface of the skin: 25 cm^2 50 x 50 mm 4 pcs./case Manufactured by: Axelgaard Manufacturing Co.,Ltd. 520 Industrial Way Fallbrook, CA 92028, USA

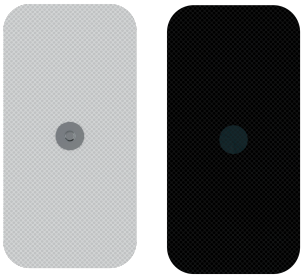	Large electrical stimulation electrode **UltraStim Snap SN2040** Area intended to contact the surface of the skin: 50 cm^2 50 x 100 mm 4 pcs./case Manufactured by: Axelgaard Manufacturing Co.,Ltd. 520 Industrial Way Fallbrook, Axelgaard 92028, USA
	Small electrical stimulation electrode **HRTC32BP** Area intended to contact the surface of the skin: 8 cm^2 dia 32 mm 4 pcs./pack Manufactured by: HUREV Co., Ltd. 107-3 Donghwagongdan-ro, Munmak-eup, Wonju-si, Gangwon-do, 26365, Republic of Korea

Meissa OT Ultra is compliant with any surface self-adhesive EMS electrodes that meet IEC 60601-1 requirements (carbon electrodes are not recommended). **Using electrodes smaller than 32 mm in diameter (with a surface area less than 8 cm^2)** may lead to burns due to the concentration of current over a smaller area. The device is designed for use with snap electrodes; using other types of electrodes requires an adapter.

Before use, always check and follow the information provided by the electrode manufacturer, paying particular attention to the maximum allowable current for electrical stimulation.


Always **confirm the use of electrodes** not listed above **with the manufacturer or the local distributor**. The use of electrodes not listed in the table above or not confirmed by the manufacturer or local distributor may result in device malfunction, failure to operate, or **pose a burn risk to the patient**.

The **size of the electrodes** should be selected **appropriately for the area** of application.

The choice of electrode is determined by the professional user, who should have the necessary knowledge to specify this. The user using the device in a home healthcare environment (lay operator) should only use the electrodes indicated by the therapist.

9.5 Transport Box

- Box where operator can put and storage device.
- Provides protection for the device during delivery and storage.
- Designed for transport from manufacturer to the client.
- Reusable.
- Hardcase is optional.

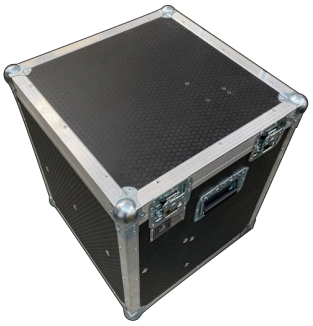

Hardcase



Carton Box

9.6 Electric Table

- Available optionally, depending on the order specifications.
- A table with adjustable height.
- Verified safe use with Meissa OT and the Arm Support accessory (described in chapter **9.7 Arm Support**).
- Equipped with measuring rulers on the front that allow for precise positioning of the Arm Support accessory to the patient's needs.
- **For professional use only.**

ESTABLISHED AND TRADE NAME

Electric Table

DIMENSIONS & WEIGHT (WITHOUT ACCESSORIES)

Total width	1150 mm
Total depth	750 mm
Total height	670-1320 mm
Total weight	max. 65 kg

ENVIRONMENT


Intended location	indoor use
Operating temperature	10°C to 40°C
Operating humidity	10% to 95% RH, non-condensing
Maximum operating altitude	3 000 m a.s.l.

MECHANICAL PROPERTIES

Speed	36 mm/s
Max table safe working load	300 kg

OTHERS

Power supply	100-240 V, 50/60 Hz, 600 W max
Protection class against electric shock	I (functional grounding)
Duty cycle operation	2 min ON, 18 min OFF

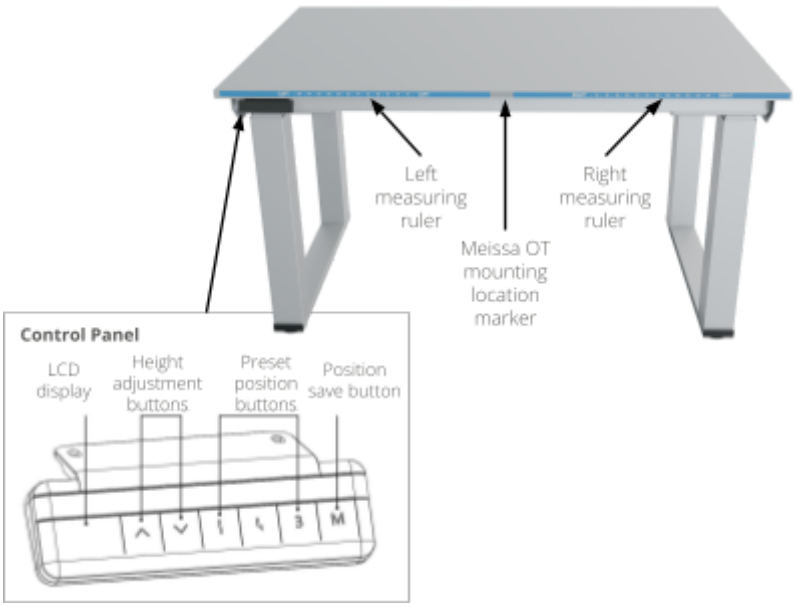

The main parts of the Electric Table are shown in the picture above.


The front part of the tabletop features blue measuring rulers on both the right and left sides, along with a grey marker that indicates Meissa OT mounting location.

The measuring rulers are designed to facilitate the positioning of the Arm Support.

The Electric Table should be positioned so that the part with the measuring rulers and control panel faces the patient. Additionally, ensure that there is enough clear space in front of the table to accommodate a wheelchair or chair.


The table should be placed on a flat, level surface.

Ensure that there are no obstacles near the table that could hinder or prevent its adjustment, as this could pose a **risk of damaging the table or the obstacles**.

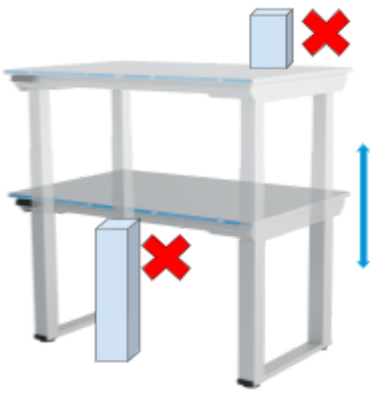

9.6.1 Electric Table use and adjustment


To mount Meissa OT on the Electric Table, follow the instructions provided in section **10.3 Platform - How to mount/dismount Meissa OT to/from the worktop**. Ensure Meissa OT is correctly positioned relative to the mounting location marker.

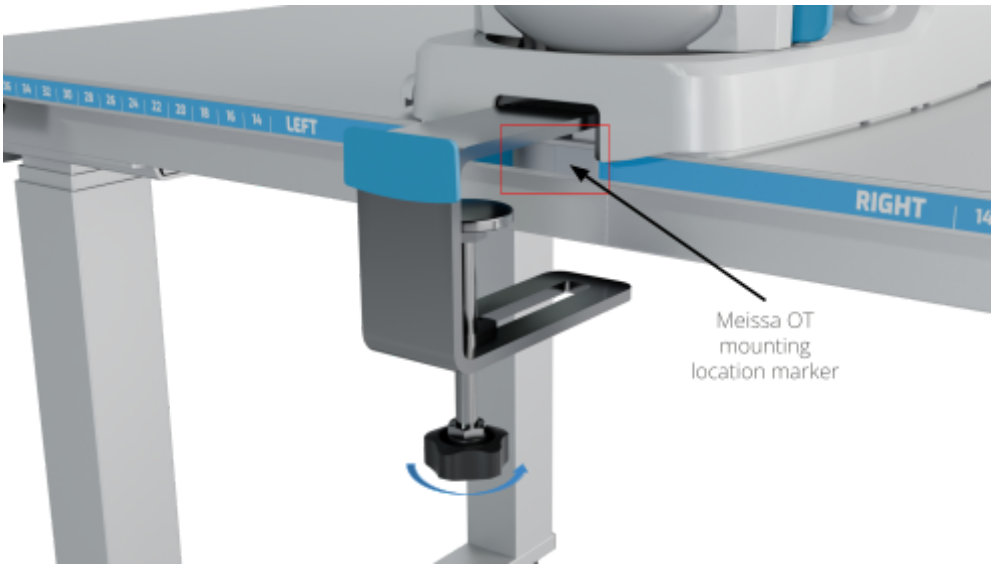

Do not attach the table mounting clamp to the metal table!

After installing Meissa OT device, ensure that **no part of the device or any of its accessories comes into contact with the metal components** of the table, cabinet, or any other object on which it has been installed before use - risk of electrical shock or burns.

The height adjustment is stepless. To **adjust the Electric Table height**, use the height adjustment buttons on the control panel. The description of the control panel elements is shown below.

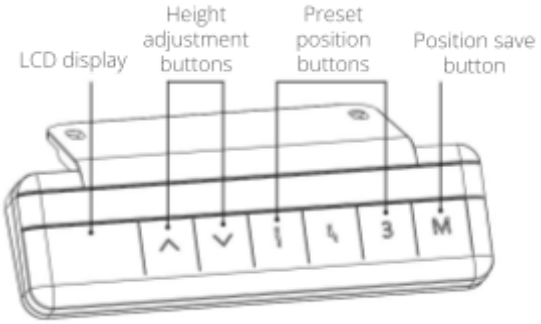

Do not adjust the height of the Electric Table during exercises or when the patient is secured to Meissa OT or the Arm Support! The risk of discomfort or injury to the patient.

The Electric Table is equipped with the ability to save three custom height positions. To save the current position, press the position save button (M). The LCD display will show "5-". Then, press one of the three preset position buttons (shown on the picture above). The current height will be saved under the selected button.


After the saving process, the LCD display will show one of the following combinations: 5-1, 5-2 or 5-3 depending on the pressed preset position button.



Once saved correctly, pressing the desired button will move the table to the saved position (only if it is different from the saved one).

The anti-collision function is responsible for detecting objects during the height adjustment of the Electric Table and will stop the movement if it encounters an obstacle. To **set the sensitivity of the anti-collision function**, press and hold the indicated buttons for 5 seconds. Then, use the height adjustment buttons (up/down arrows) to set the sensitivity:

- A-0 Anti-collision function disabled
- A-1 Low sensitivity
- A-2 Medium sensitivity
- A-3 High sensitivity

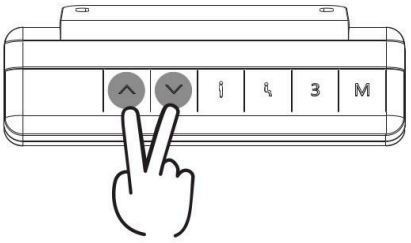

9.6.2 Troubleshooting

Reset function: When the display shows "A5R" or "rSE", press and hold the down button until the Electric table moves to the lowest or highest position after the rebound stop. At this time, the display will show the height figure. Release the down button, the reset is complete, the table can be used normally.

If the "E01" or "E02" appears, please let the table rest for more than 18 minutes, before using it normally.

For other error codes, press the down button to reset the table.

If there is still no response, ensure that the connection cable is intact and properly connected. Power off the table for more than 10 seconds, then reconnect the power. When the display shows "A5R" or "rSE", press and hold the down button to reset.

If the table still does not operate normally after performing the above steps, please contact the customer service.

Malfunction	Solution
The table does not respond to button presses.	Check the connection of all cables.
The table raises slowly.	Check if the load does not exceed the maximum safe working load of 300 kg.
The table lowers unintentionally.	
The table resets automatically.	
The table raises but does not lower (or vice versa)	Reset
The height adjustment range is incorrect.	
The table does not raise.	
The actuator system has been overloaded (exceeded the work cycle: max 2 min work for 18 min break).	Allow the system to cool down for 18 minutes, then reset it.
Pressing the "down" height adjustment button raises the table.	Ensure the height adjustment range of the table is clear of obstacles.

9.7 Arm Support

- Available optionally, depending on the order specifications.
- Designed to provide continuous support for the patient's upper limb during training on Meissa OT device.
- Adjustments allow for setting the height and positioning the limb in the transverse plane (horizontal) relative to Meissa OT.
- Equipped in the interchangeable cushions for supporting the wrist or forearm, along with straps to secure the patient's limb.
- It's recommended to use the Arm Support accessory in connection with a dedicated table to achieve the best fit for the patient.
- The Arm Support can be used on patients over 3 years of age, but make sure that it does not generate hazards and that it is suitable for the size of the patient's limb.
- **For professional use only.**





The Arm Support set is designed to support the upper limb (right or left) and to fix it in a set position on a horizontal plane relative to Meissa OT, with adjustable height from the mounting surface.

The device consists of five components:


- Cushion small (1),
- Arm support (2),
- Table clamp right (3),
- Table clamp left (4),
- Cushion large (5).

The accessory allows for the positioning of the wrist support cushion (cushion small) or forearm support cushion (cushion large) in a position tailored to the patient. For this purpose, the positions of individual elements can be adjusted or locked using dedicated knobs. Additionally, indicators placed near the movable joints allow for precise adjustment of the Arm Support.

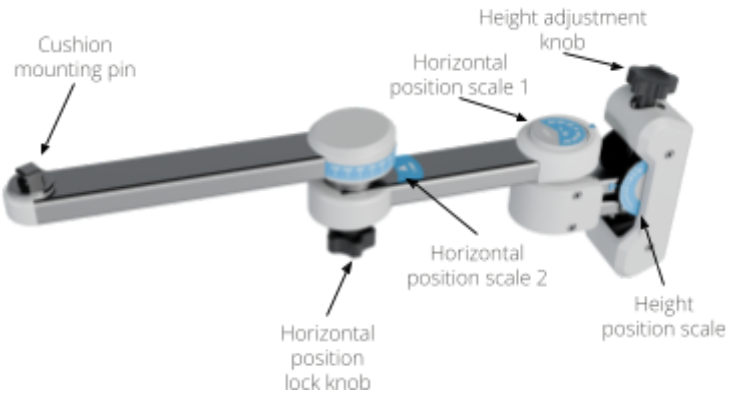

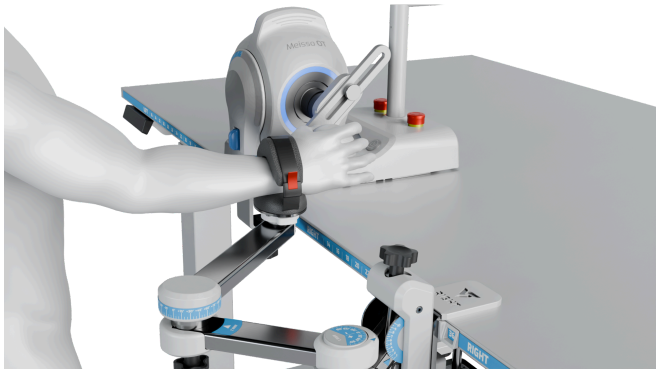

Proper support of the wrist on a small cushion.

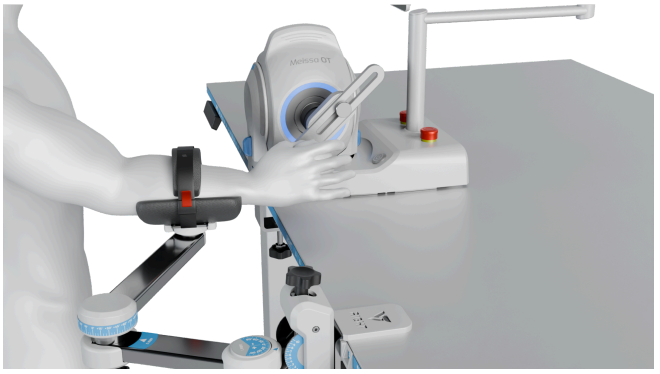

Proper support of the forearm on a large cushion.


The table mounting clamps are labeled to indicate the intended sides for installation.




The Arm Support contains clamps and straps to secure the limb, other methods of stabilising the limb (e.g. elastic bandages) should not be used. The use of improvised or non-approved fixing methods, may delay emergency response and pose a risk to patient safety.

9.7.1 Arm Support assembly

The table clamps (right and left) should be mounted on the respective sides of the device. To install the clamps, loosen the knob, position the clamp against the front edge of the tabletop, and then tighten the knob securely.
The table mounting clamps can be attached to surfaces with a thickness ranging from 10 to 40 mm.

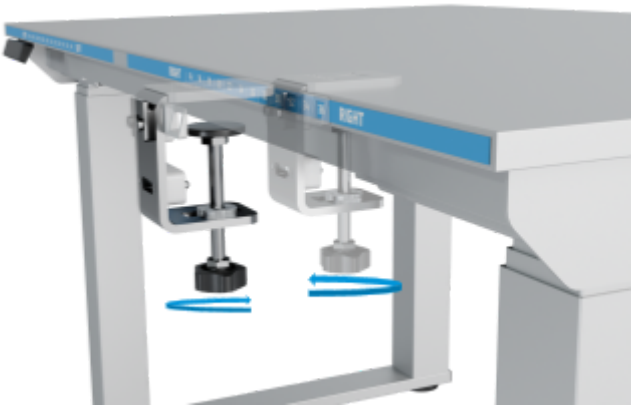



After mounting the clamps, ensure they are securely tightened. Check that the clamps are flush against the front edge of the tabletop and that the rubber part of the knobs is pressed against the underside of the tabletop.

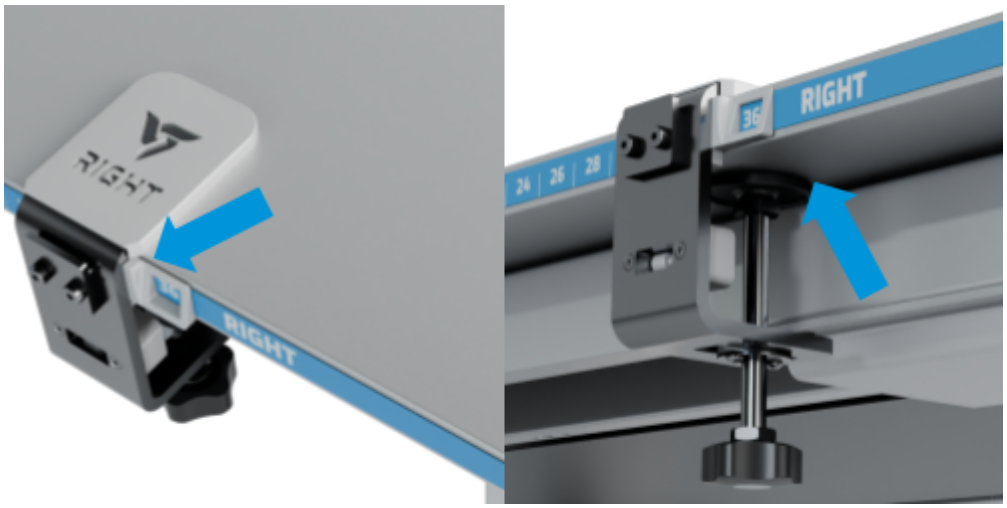


Always ensure that the table clamps are correctly installed. Improperly mounted clamps pose a risk of accidents and potential **injury** to the patient or therapist.

To secure the Arm Support, align it at an angle above the selected table clamp so that the positioning pin is inserted into the mounting hole in the table clamp, as shown in the pictures below. Then, press it firmly onto the clamp surface.

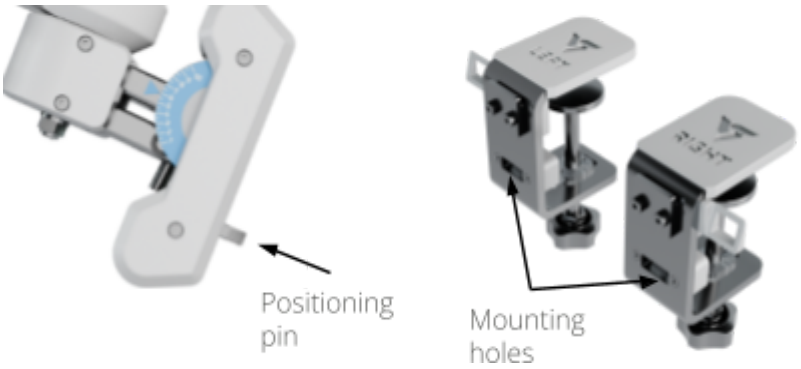

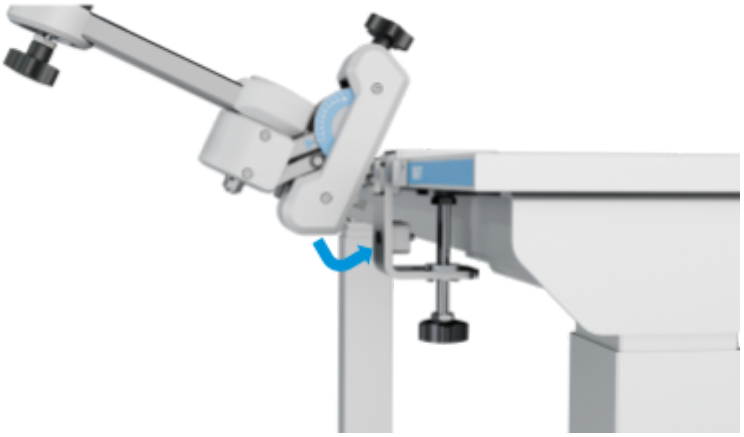


A correctly mounted Arm Support fits snugly against the table clamp.

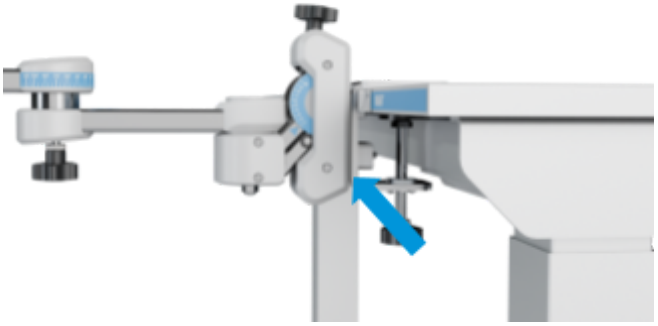

The Arm Support should always be mounted on **clamps that are securely attached to the table!**

Before using the Arm Support, attach the appropriate cushion suited to the therapy needs – use the small cushion for wrist support or the large cushion for forearm support. To mount the cushion, press buttons 1 and 2 on the cushion, then place it onto the mounting pin.

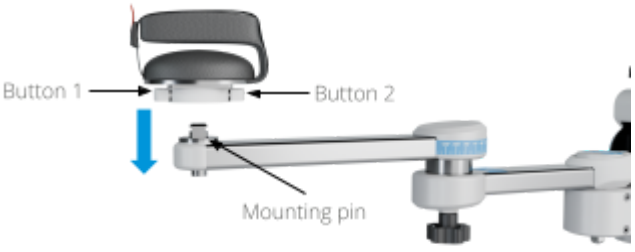

Correctly mounted support cushion.



Height adjustments range from the table surface to the Arm Support are: 8 to 14 cm for wrist cushion and 10 to 16 cm for forearm cushion.


Before use, ensure that the cushion, clamp, and Arm Support are correctly mounted, with the Arm Support securely attached to the clamp and the clamp firmly fastened to the tabletop.

Do not use the accessory if any part is missing!


9.7.2 Arm Support use and adjustment

Before using the Arm Support, adjust its position to suit the patient's needs and the exercise being performed. Ensure that the Arm Support is correctly mounted on the table clamp on the appropriate side (right or left), and that the chosen cushion is properly attached to the Arm Support.


Next, position the table clamp at the appropriate distance from Meissa OT. To do this, loosen the knob on the selected table clamp, move the Arm Support along the tabletop to the desired position, and then tighten the table clamp knob. **Ensure that the clamp is properly mounted!**

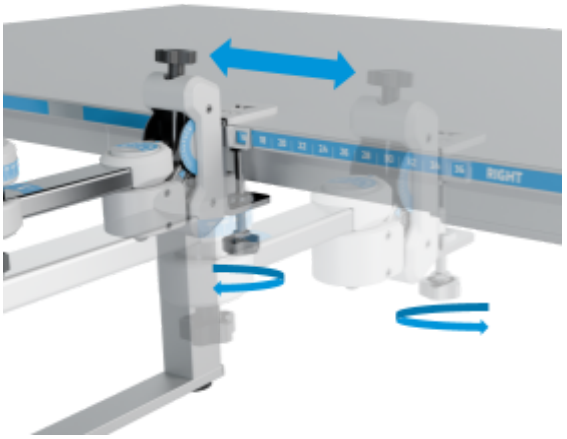

Using the height adjustment knob, set the required height of the support. The adjusted height can be verified on the height adjustment scale.

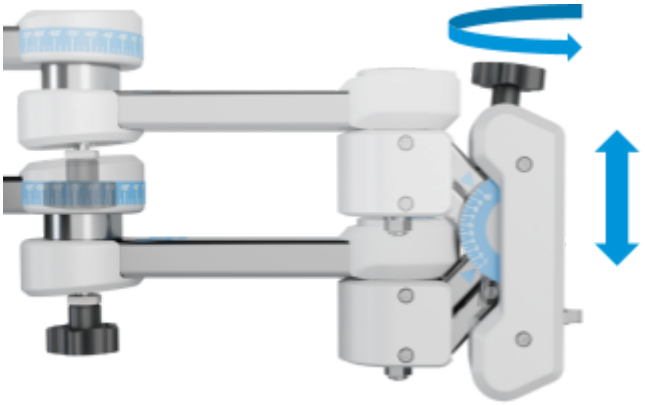

To set the position of the Arm Support on the horizontal plane, loosen the horizontal position lock knob, adjust the Arm Support to the desired position, and then fully tighten the knob again. **The user expects full fixation of the Arm Support by tightening the underside knob, but the mechanism only partially restricts movement.**

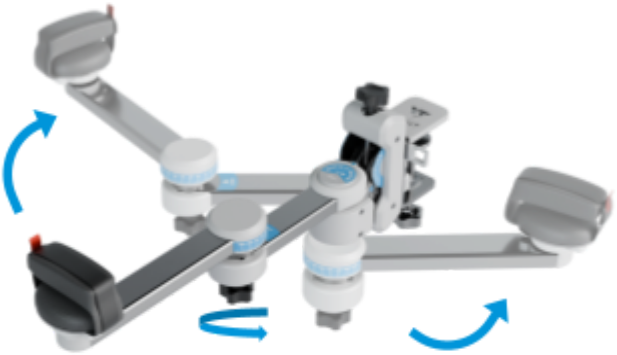

Both supporting cushions are equipped with straps for securing the patient's upper limb if there are no contraindications (e.g. spasticity). Before starting exercise, fasten the patient's wrist or forearm. Ensure that the straps are adjusted to fit the size of the patient's upper limb.

Height adjustments of the table or the Arm Support must be performed without the patient secured to Meissa OT or the armrest. The fixation of the upper limb (to either the Arm Support or Meissa OT) should only be done once the appropriate height for the exercise is set and will no longer be adjusted.


Do not adjust the height of the table or the Arm Support during exercises or when the patient is secured to Meissa OT or the Arm Support!

Before use, ensure that the Arm Support is correctly mounted and all components are properly installed.

Do not use the accessory if any part is missing!

During adjustment procedures, there is a **risk of hand injury**. Pay special attention to the limbs of both the operator and the patient while setting up the Arm Support.



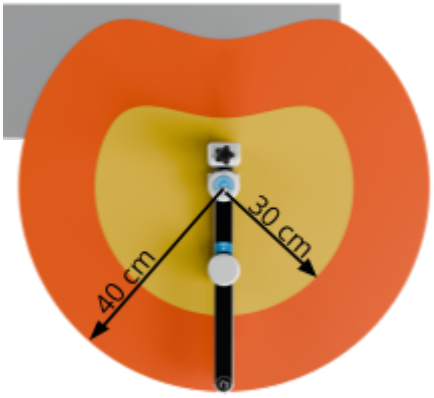

The maximum safe working load for the Arm Support is **5 kg** in its fully-extended position (marked in orange above) and **10 kg** in half-extended position (marked in yellow above).

However, be aware that applied load may cause damage to the tabletop, on which the Arm Support is mounted. Therefore, **always pay attention to the Arm Support and the tabletop during use** to prevent potential damage and injury.

During electrical stimulation (Meissa OT Ultra only), **ensure that neither the patient nor the therapist touches the Arm Support**. Only the patient's upper limb should rest on the cushion (either small or large) and be secured with a strap.

Do not attach the Arm Support and Meissa OT to the metal table! Fixing the Arm Support is only allowed to the non-conductive surface of the table top.


After installing Meissa OT device, before use, ensure that **no part of the device or its accessories touches the metal components** of the table, cabinet, or any other object on which it has been installed - risk of electrical shock or burns.

Before starting the exercise, check that there will be no collision between the Arm Support, the device, the extension and other objects or accessories when the limb is secured in the support with the straps.

10. Basic information about Meissa OT

10.1 How is Meissa OT built

Meissa OT and its user interface are shown below.

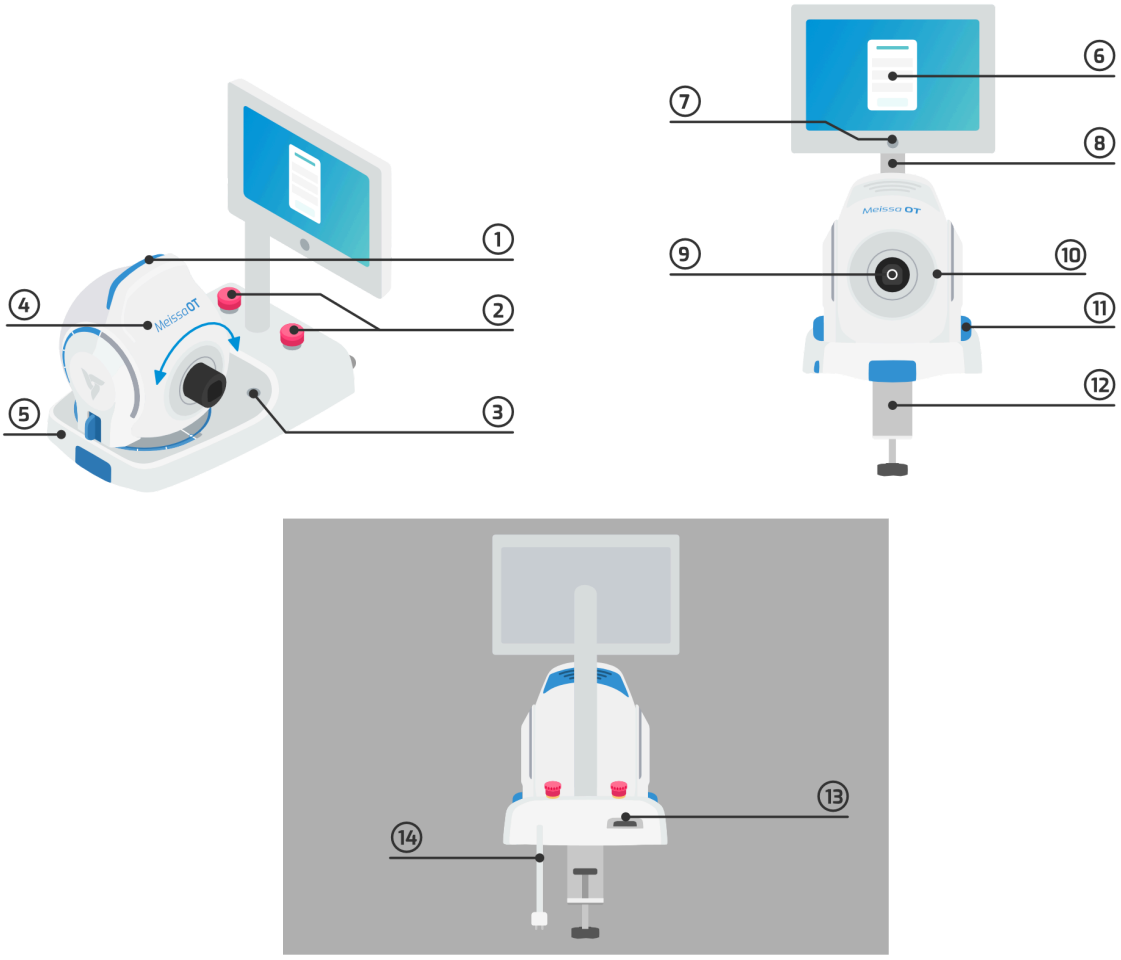

No.	Name	Operation description
1	Vertical position lock button	Adjusting the head's vertical position
2	Emergency stop push buttons (Emergency buttons)	Stop all movement of Meissa OT by cutting off the motor power supply. Emits a sound notification when applied (described in 10.7 Sound notification)
3	Power switch	Allows to turn the device on or off
4	Head	Device working part, can be rotated in relation to the platform horizontally and vertically

5	Device platform	With mounting system, fixed to the tabletop
6	Touchscreen display	It is used to display software and operate the device
7	Touchscreen display button	Displays motor lock option
8	Tablet holder	Allows to position the tablet to accommodate different patient positions
9	Extension socket	Allows you to connect extensions available for the device
10	LED ring	Displays visual notification during use (described in **10.6 LED Ring - Visual notification**)
11	Horizontal position lock button	Adjusting the head's horizontal position
12	Table mounting clamp	Securely attaches the device to the table, prevent the device from sliding on the table during patient use
13	EMG/EMS cable port	Allows to connect an EMG/EMS cable
14	AC power supply cable	Supplies power to the device
15	AC power supply cable port (not visible)	Allows to connect an AC power supply cable
16	Extensions (not visible above, described in **9.1.1 Extensions**)	Allows for the evaluation and exercise of various hand and finger movements
17	EMG/EMS cable (not visible above, described in **9.2 EMG/EMS cable**)	Used for transmitting electromyographic (EMG) signals and muscle stimulation (EMS)
18	EMG electrodes (not visible above, described in **9.3 Electrodes for surface electromyography (Meissa OT Ultra only)**)	Detects and transmits electromyographic (EMG) signals from muscles
19	EMS electrodes (not visible above, described in **9.4 Electrodes for electrostimulation (Meissa OT Ultra only)**)	Delivers electrical stimulation to muscles
20	Electric Table (not visible above, described in **9.6 Electric Table**)	A table with adjustable height for optimal device positioning
21	Arm Support (not visible above, described in **9.7 Arm Support**)	Provide continuous support for the patient's upper limb during training
22	Software - EGZOClinic Application (not visible above, described in **17. Programs Overview**)	Allows to operate the device

10.2 Technical Specifications

ESTABLISHED AND TRADE NAME

Meissa OT

DIMENSIONS & WEIGHT (WITHOUT ACCESSORIES)

Total length	347 mm (transport position)
Total width	294 mm (transport position)
Total height	485 mm (transport position)
Total weight (except extension)	max. 13 kg

PATIENT SIZES

Patient weight	max 150 kg
Arm weight	max 8.6 kg
Patient age	min 3 y. O.

ENVIRONMENT

Operating temperature	10°C to 40°C
Operating humidity	10% to 95% RH non-condensing
Maximum operating altitude	3 000 m a.s.l.
Cooling	convectional
Ingress protection (IP code)	IP21
Mobility	portable
Operation type	continuous, software controlled

MECHANICAL PROPERTIES

Rotation speed	120 deg/s
Drive rotation	continuous (unlimited)
Torque	16 Nm
Torque measurement accuracy	± 0.05 Nm
Vertical rotation range	-90° to +90°
Vertical rotation step	15°
Horizontal rotation range	0° to +90°
Horizontal rotation step	15°
Goniometer measurement accuracy	± 2°

ELECTROMYOGRAPHY (Meissa OT Ultra only)

Electromyography measurement channels	up to 4 simultaneous sampling
Baseline noise	< 0.5 µV RMS
Input-referred noise	10 µVp-p (10 s of raw data)
Measuring Voltage range	-0.6 V to 0.6 V
Meissa OT Ultra's gain	1
Sampling frequency	up to 1 000 samples/s per channel
Internal resolution	24-bit
CMRR	-73 dB
Input impedance	10 MΩ
Electromyography accuracy:	± 0.5% full scale

ELECTRICAL STIMULATION (Meissa OT Ultra only)

Electrical stimulation channels	up to 4, sequential
Waveforms and types	low-frequency, dual-phase and direct current free rectangular, triangular, and trapezoidal pulses, electromyography-triggered
Maximum output voltage and current	50 V / 100 mA at 500 Ω

PULSES PARAMETERS

Pulse frequency	5 - 100 Hz
Pulse width	50 - 500 µs
Rise time	0 - 4 s
Plateau time	1 - 20 s
Fall time	0 - 4 s
Waveform generation accuracy	± 0.5% full scale
Output resolution	16-bit
Sampling frequency	up to 1 000 000 samples/s
Load impedance	500 - 2000 Ω

FORCE SENSOR PARAMETERS

Used in	pinch meter
Measurement range	0 - 100 N
Measurement accuracy	± 0.25 N

OTHERS

Power supply	100–240 V, AC 50/60 Hz
Current required	max 0.7 A at 240 V max 1.5 A at 100 V inc. tablet
Fuses type used	4A (T4AL250V)
Protection against electric shock	class I grounded/earthed (⏚) connection required
Applied part type	BF
Communication interfaces	wired (USB) and wireless (Wi-Fi, Bluetooth)

ARM SUPPORT SAFE WORKING LOAD

Arm Support in half-extended position	max 10 kg
Arm Support in fully-extended position	max 5 kg

10.3 Platform - How to mount/dismount Meissa OT to/from the worktop

Meissa OT has a platform for attaching the device to the tabletop. To secure the device to the tabletop, use the table mounting clamp described in chapter **9.1.3 Table mounting clamp**. The device can be securely mounted to the tabletops with thicknesses from 5 mm to 60 mm.

Before starting any training program, be sure to securely attach the device to the tabletop.


The table, cabinet, or furniture with a **worktop** on which Meissa OT will be mounted should be placed on a **flat, level surface.**


A tabletop with a thickness of less than 18 mm that is not supported from below by a steel frame **may break during the use** of Meissa OT, posing a **risk to both the patient and the operator**. It is recommended to use tabletops with a thickness greater than 18 mm.

To mount Meissa OT on a table, cabinet, or other worktop, position Meissa OT so that the protruding part of the platform extends beyond the front edge of the surface. Next, ensure that the securing knob on the table mounting clamp is loosened.



Then, place the table mounting clamp into the slot at the front of the device, ensuring that it is fully engaged with the device.

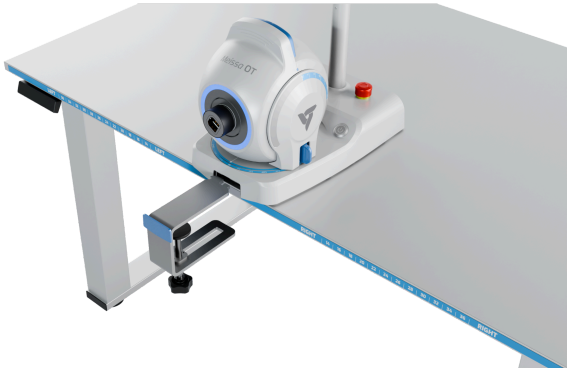

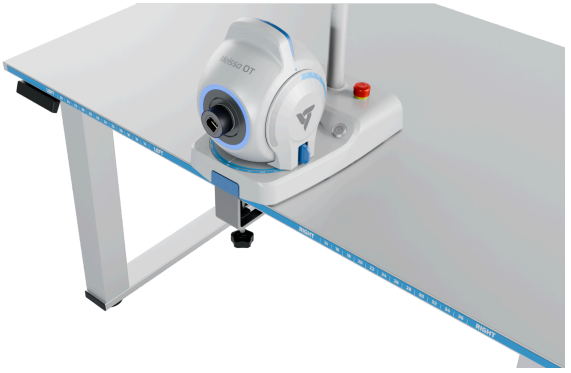


Next, tighten the securing knob on the table mounting clamp fully against the worktop, ensuring that Meissa OT is securely attached and that no movement is possible. To tighten the securing knob, tighten it by hand until resistance is felt.



The drawings below illustrate **the most common incorrect methods for mounting Meissa OT**. Ensure that none of these errors have been made.





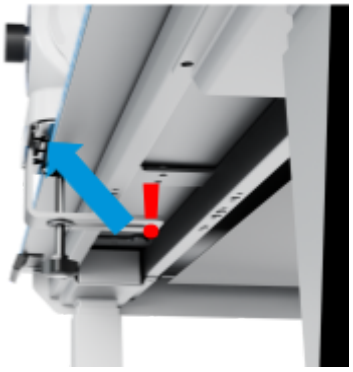

Meissa OT's platform has two ports located on the back of the platform. One is for AC cable, and the second is for EMG/EMS cable (Meissa OT Ultra only).


Always use only the compatible AC cables and fuses according to electrical requirements listed in chapter **10.2 Technical Specifications**.

The connection ports of Meissa OT's Head are intended for specific accessories mentioned above. **Do not connect any other devices to those ports!**

Do not attach the table mounting clamp and Meissa OT to the metal table!

After installing Meissa OT device, before use, ensure that **no part of the device or its accessories touches the metal components** of the table, cabinet, or any other object on which it has been installed - risk of electrical shock or burns.


To dismount Meissa OT from the worktop, unscrew the securing knob, unlock the clamp with the side button, marked with an information sticker, and remove the table mounting clamp. The securing knob may require high torque to loosen.

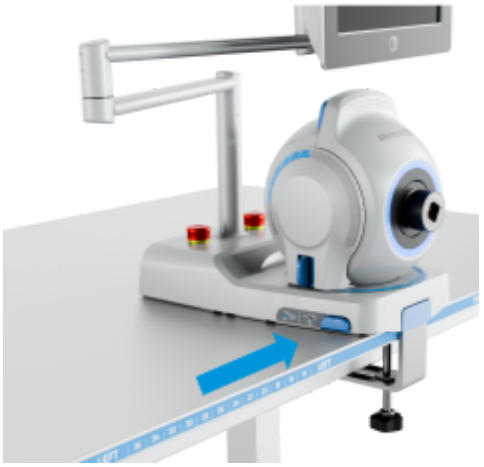

10.4 Head - Adjustment of Meissa OT in the vertical and horizontal planes

The main part of the device (head) can be rotated horizontally in relation to the platform in a range of -90° to 90° and vertically in the range of 0° to 90° in 15° increments.

To adjust the **head's vertical position,** press the blue button located at the top of the device (shown below) and holding it down, move the head to the desired position. Releasing the button will lock the head in place.

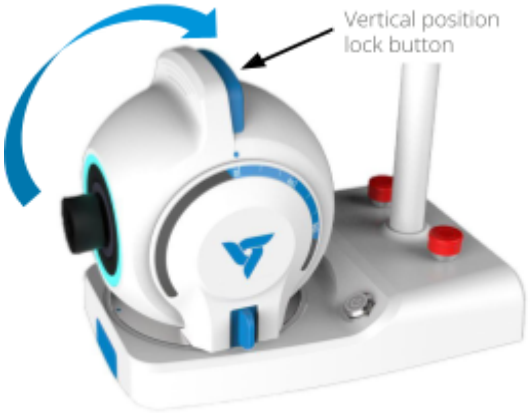

To adjust the **head's horizontal position**, press the blue buttons located on the right and left sides of the device near the platform, and while holding them down, move the head to the desired position. Releasing the buttons will lock the head in place.



Press the position lock buttons with sufficient force. Do not turn or yank the head if the lock has not been released. After releasing the buttons, check the proper alignment of the head and the activation of the lock.

Meissa OT has **four extension connector pins** located on the front of the Head. Those connectors are used to power the extension. While working with Meissa OT, **your patient should not touch these connectors**, either directly or indirectly through you **(the patient should not touch the supervisor while they are touching these connectors)**.

10.5 Tablet holder - Adjustment of the tablet position

The tablet holder has integrated cable with the DC output to the tablet's power adapter and data transmission. The tablet's position can be adjusted to accommodate different patient positions. Be sure to leave sufficient mounting space for the tablet holder to move to avoid, for example, collision with a wall.


The best therapy position for the tablet is in front of the operator's and patient's eyes (if it is important that the patient can see the screen during therapy, e.g. while game playing), the tablet should not be in conflict with any other object.

To set the tablet in the desired position, grasp the tablet and adjust it as needed. It is possible to adjust the horizontal position of the tablet along with adjusting the tablet angle.

The device must be operated in a working area with adequate lighting levels to ensure safe use of the robot. The lighting must provide adequate visibility of the device to the patient and user, including visibility of the contents of the control tablet screen.

The cable integrated into the tablet holder is intended for a specific 10" touchscreen tablet that is inseparable from Meissa OT, has the application installed and is supplied by the manufacturer with Meissa OT. **Do not connect any other devices to this cable!**

When adjusting the tablet's position, be aware of the **risk of hand injury**.

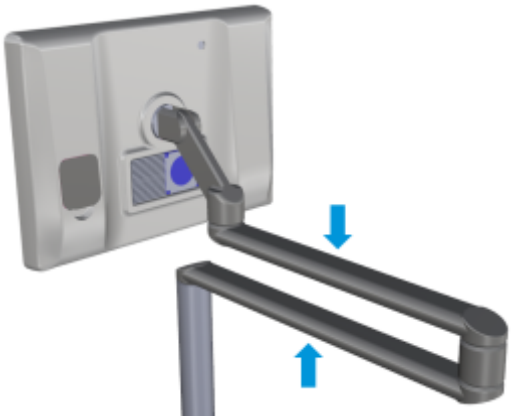


The use of the tablet holder as a support when standing up is unacceptable and may cause damage to the device or injury to the patient.

10.6 LED Ring - Visual notification

Meissa OT device emits only one visual (light) informative notification when powered on, as indicated in the table below. The information provided by the LED ring is neither critical nor essential, as the user can verify whether the device is powered on through the touchscreen display's operation.

The device does not generate visual errors or warnings notifications.

The LED ring's purpose is more decorative than functionally significant.

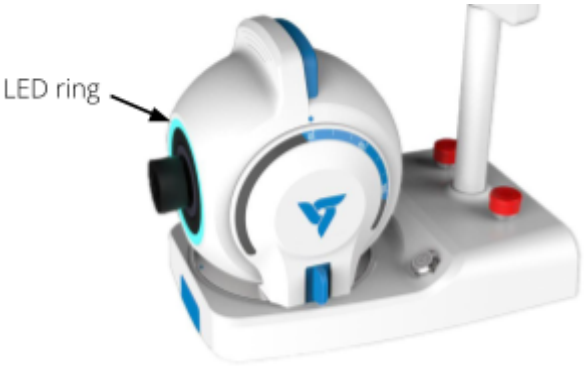

Description	Operators Activity	Status
The LED ring lights up in blue with a green point	This occurs after pressing the power button if the device was turned OFF	**The device is turned on. When turning ON, the green point indicates the extension's position***
The LED ring is not lit	This occurs after pressing the power button if the device was turned ON	**This indicates the device is turning OFF**

* The exact position of the extension is provided within the software, which displays this information. Therefore, the green point serves primarily a decorative or supportive function rather than providing essential information for the user.

10.7 Sound notification

Meissa OT device emits only one sound informative notification. It is emitted when one or both of the Emergency stop push button(s) (Emergency button(s)) is/are applied, indicating that the emergency stop push button is/are in force. This is a repetitive, specific sequence of tones with fixed parameters, selected for good audibility. Sound stops as soon as the activated Emergency button(s) is/are deactivated.

In addition to the sound notification, the device displays a notification on the touchscreen display indicating that the Emergency stop push button is active (described in detail in chapter **14. Notifications, Information, Errors, and Warnings displayed by the Software**). The sound notification is additional, and it is not understood as an alarm in the context of the IEC 60601-1-8 standard, as it is intended solely to indicate the activation of the emergency stop push button and not to signal a critical error.

The device does not generate sound errors or warnings notifications.

10.8 Typical issues

Anyone who attempts to repair and/or modify Meissa OT and/or its accessories risks damaging Meissa OT and/or accessories. Therefore, any steps not described in the troubleshooting guide (table below) are prohibited. Improper use voids all warranty claims.

Problem	Possible Cause	Solution
Meissa OT does not turn on	AC cable plugged incorrectly	Replug the AC cable
	AC cable not plugged	Plug in the AC cable
	Power switch turned off	Turn the power switch on
Meissa OT does not detect the extension	Extension plugged incorrectly	Firmly replug the extension
Weak electrostimulation	Dried out or damaged electrodes	Replace and re-connect electrodes
	Incorrect electrode placement	Replace and re-connect electrodes
	Worn or damaged lead wires	Replace leads
Intermittent EMG signal	The electrode lead set is loose or disconnected	Check the lead set connections in both Meissa OT and electrodes
	Electrodes dried out or damaged or were not in contact with bare skin	Change the electrode to a new one
The EMG signal cannot be controlled	The electrode or reference cable is not connected properly	Check and improve connection of electrode or reference cable
	The electrode lead set is loose or disconnected	Check the lead set connections in both Meissa OT and electrodes

Problem	Possible Cause	Solution
The EMG signal cannot be controlled	Electrodes dried out or damaged or were not in contact with bare skin	Change the electrode to a new one. Ensure if the skin is properly prepared
Meissa OT does not move	Device's drive malfunction	Contact with **EGZO**Tech service request form is available at: https://service.egzotech.com
Meissa OT stops operating during use	A temporary mains power interruption has occurred (e.g. lasting 5 seconds or longer).	The device does not resume operation automatically after power is restored. To restore normal operation: 1. Ensure that mains power has been restored and is stable. 2. Switch the device OFF using the main power button. 3. Switch the device ON again using the main power button. 4. The Meissa OT device will restart automatically and display the login screen. 5. Log in and re-enter all exercise parameters, including patient-specific settings, program, intensity level, and other required values. Failure to follow these steps may result in improper device operation or loss of saved therapeutic settings.

10.9 Emergency stop push buttons

The emergency stop buttons are located on Meissa OT platform. It can be pushed by the therapist and the patient in case of any danger occurs.

Meissa OT has two emergency stop buttons that will stop all movement of Meissa OT by cutting off the motor power supply.

The emergency stop buttons are only used to interrupt therapy or operation of the device in patient and emergency situations and must not be used in normal operation and in the absence of hazards.

The device remains in the emergency stop state until both buttons are released. If even one of the buttons is used during the exercise, the device circuits are switched off and therapy is interrupted.



Emergency stop buttons do not switch off the power to Meissa OT entirely. In the event of a fire, water spill, or any other non-mechanical malfunction, step away from Meissa OT as soon as possible.


Emergency stop
buttons

11. Extensions

Extensions are interchangeable accessories for Meissa OT that are mounted on the front of Meissa OT's Head and are responsible for performing training exercises.

The extensions enable joint movement with specified force resistance (or assistance). These are the components that will most often move (or be moved by) your joint.



The use of improvised or non-approved limb fixing methods (e.g. elastic bandages), may delay emergency response and pose a risk to patient safety. If such methods are used, ensure they allow for **quick release of the limb**.

11.1 What kind of extensions do I have?

All extensions provided with Meissa OT are listed in chapter **9. What will I find in the package?**


There is an occupational therapy extension - the pinch meter - which can measure grip force. This extension can be rotated during movements imitating activities of daily living.

11.2 Plug in/out your extension


All extensions are plugged as shown below.

Place the extension on the front of the socket, paying attention to the key slot shape.


Insert it into the socket until a "click" sound is heard.

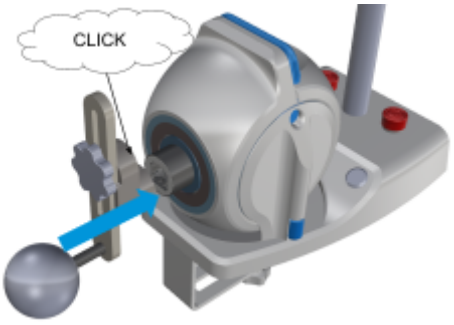

The extension is properly plugged into the device socket.

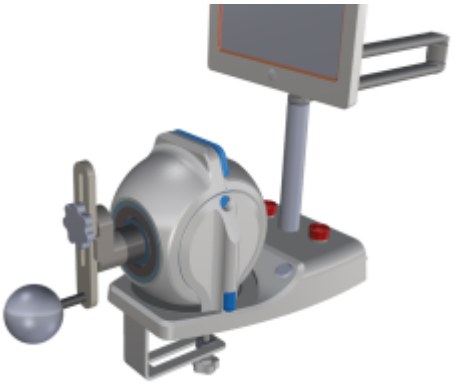

To unplug extension, hold the socket latch (red indicators) and push it in the opposite direction with sufficient force until it is completely removed from the socket.

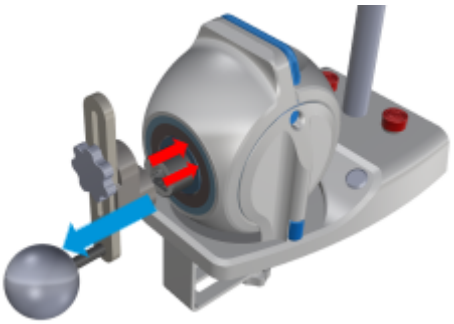

When mounting the extension, it must be pressed down with sufficient force, causing the extension to lock into the socket. An improperly pressed extension is not detected by the robot, causing the robot to lock and preventing the treatment from taking place. After mounting, verify the correct installation of the extension in the socket.

Do not adjust the height of the table or any **accessories** during exercises or **when the patient is secured to Meissa OT or the Arm Support!**

12. Electromyography (Meissa OT Ultra only)

12.1 How it works

Electromyography is an electrodiagnostic medicine technique for evaluating and recording the electrical activity produced by skeletal muscles. The signal originates from the depolarisation of the motor units and muscle fibers by the action potentials (signals generated in our motor cortex, going through the spinal cord and into skeletal muscles). The more motor units get activated simultaneously during muscle contraction, the higher the amplitude of EMG RMS signal.

Meissa OT Ultra was designed to allow bioelectric measurements, particularly for diagnostic and reactive electromyography. In Meissa OT Ultra's package (described in chapter **9. What will I find in the package?**), you will find an EMG/EMS cable and electrodes for surface electromyography.




Meissa OT produces results that are informative, not diagnostic. Qualified individuals must interpret these results.

12.2 Lead wires and channels for EMG

The cables have color-coded snaps for each of the differential EMG channels:

Color	Channel name
Red	Channel 1
Blue	Channel 2
Green	Channel 3
Purple	Channel 4
White	Reference

Each lead wire for the EMG has a colored snap to connect the EMG electrode. Two snaps of the same color correspond to one channel. The two color-coded snaps of each EMG channel represent two differential inputs: positive "+" and negative "-". **For electromyography, it is essential to connect both positive and negative inputs of one channel to the same muscle** (the one being assessed).

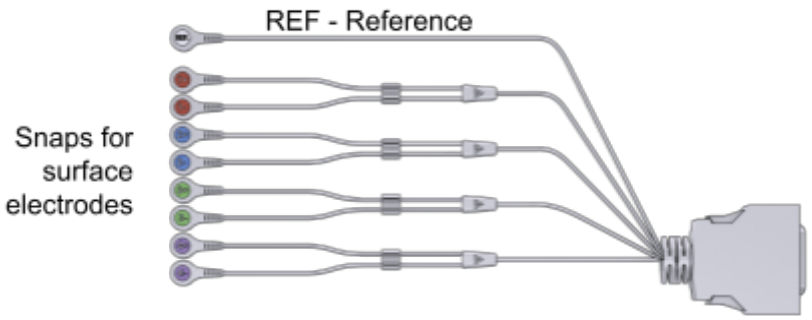

You should always have a reference input for electromyography close to the currently used EMG channels. The closer the reference electrode is to the measured channel, the less electromagnetic interference there will be. For example, try to place the reference electrode on the same limb as the measured channels.

For each EMG program (whether for data collection for diagnostic purposes or therapeutic use), you will need at least three connected electrodes: two of the same color connected to one channel and one white reference electrode.

Electromyography and electromyography biofeedback can be safely used by any user - patient or therapist alike.

There's more! Visit our website for the latest available courses!
https://support.egzotech.com

12.3 Electrodes

For differential channels (positive "+" and negative "-"), to ensure reliable training-to-training comparison of results the manufacturer advises using electrodes with a fixed distance between the electrode snaps (e.g. 2 cm).

Do not use any unauthorized electrodes, especially those lacking the necessary safety certificates.



Use only EMG electrodes approved by the **EGZO**Tech.

Never use the single use electrodes more than once, and never on more than one patient.

- We recommend using single-use snap electrodes compatible with the EMG cable.
- For reference electrodes, you are free to use any single-use electrode, although the manufacturer recommends using electrodes provided by **EGZO**Tech, which can be ordered from your product specialist or **EGZO**Tech representative.
- To achieve the best results when working with Meissa OT Ultra, we recommend using electrodes with wet gel.
- Do not use any unauthorized electrodes, especially those lacking the necessary safety certificates (medical device CE in the European Union).
- Never use single-use electrodes more than once, and never on more than one patient.
- Reusable electrodes can only be used by one patient.

12.4 EMG Electrode placement and configuration


Because electromyography is connected to motor unit action potentials and the depolarization of muscle fibres, several factors influence the reliability of EMG signal acquisition, including:

- Electrode-specific factors:
    - Area and shape of the electrode detection surfaces, which determine the number of active motor units and innervated muscle fibres. The same type of electrodes should be used to compare different results.
    - Distance between the electrodes, which determines the bandwidth of the differential electrode configuration. This distance should be constant for each measurement.
- Location of the electrode with respect to the motor points, which affects the amplitude and frequency characteristics, as well as comparability between a series of measurements. The further the electrode is from the motor point, the more the amplitude decreases,

- Crosstalk with other muscles due to close proximity of the electrode positions. Electrodes should be placed in the middle of the belly and away from the lateral edge. For smaller muscles, crosstalk should be considered during result interpretation,
- Orientation of the bipolar configuration of the electrodes with respect to the muscle fibres, which affects the measured conduction velocity, amplitude, and frequency of action potentials (depolarisation of muscles).

Follow the steps below to maximize reliability, sensitivity and accuracy of your electromyography measurements.

1. Remove hair from the patient's skin in the application area, when necessary. Clean the area with appropriate cleaning and disinfecting agents.
2. Always use **EGZO**Tech approved electrodes listed in this User Manual, as electrode properties like gel type, conductivity, and snap dimensions can greatly influence measurements.
3. Connect the EMG/ECG surface electrodes to the lead wires **before** attaching them to the patient's skin. Connect the electrodes marked blue to the snaps of the same colour and the electrode marked gray to the reference lead wire (with the REF sign).

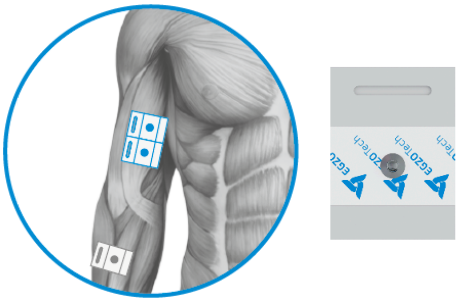

4. Select a muscle you want to measure.
5. Place the first electrode on the center of the muscle.
6. Place the second electrode adjacent to the first electrode, along the muscle fibres, so that the distance between the electrodes is consistent each time.
7. Place the **reference electrode (marked gray)** with the white lead wire ending and REF sign to the skin that is not under evaluation.
8. Ensure that electrodes are placed on dry and clean skin.

Remember to put the reference electrode on skin outside of the trained muscle. If you're using more than one channel, be sure to select muscles for each channel.

13. Electric stimulation (Meissa OT Ultra only)

13.1 Basics of electrical stimulation



Electrical stimulation should **only be used after receiving training from a healthcare professional.**

Always consult your physician before using electrical stimulation, to ensure the correct output parameters and program are selected for you. Improper selection of electrostimulation parameters can result in patient ailments due to excessive electrostimulation or a lack of therapeutic effects due to insufficient electrostimulation.

Electrical stimulation induces muscle contraction by conducting an electric current through the muscle fibers of the targeted muscle. It mimics the signals sent from the nervous system.

The electrical stimulation programs in Meissa OT Ultra include:

- **EMS programs** - These programs enable electrical stimulation of the motor neurons.
- **EMG-triggered EMS** - This involves initiating a voluntary contraction for a specific movement. Once the muscle activity reaches a pre-set threshold level, and then an assisting electrical stimulus is applied.

Refer to section **7.4 Electrical stimulation safety, including TENS (Meissa OT Ultra only)** before starting work.

13.2 Lead wires and channels for EMS

For electrical stimulation, you should use two outputs from one channel: positive ("+") and negative ("-"), corresponding to two lead wire snaps of the same color.

When leaving loose cables while using fewer channels than provided by the EMG/EMS Cable the unused channels and their lead wires should be protected against mechanical damage, especially in contact with moving parts of the device. It should also be ensured that the lead wires are electrically separated from the patient, the user, metal components of the device with accessories and other objects with which the snap could come into contact.

13.3 EMS Electrode placement and configurations

In Meissa OT Ultra, a two-electrode electrical stimulation method is used. This technique involves placing two electrodes of equal size on the skin, positioned where the muscle transitions to the tendon. This method is typically used for the electrostimulation of denervated muscles. However, the two-electrode method can also yield good results when used to stimulate healthy or mildly damaged muscles to contract.



Use only electrodes authorized by **EGZO**Tech, as described in chapter **9.4 Electrodes for electrostimulation**. **Using electrodes that are the wrong size or not suited for the application could lead to skin reactions or burns**. Electrode properties, such as dimensions, conductivity, impedance, and connector types, can greatly impact safety. **Never use ECG/EMG electrodes for electrical stimulation.**


In bipolar electrode placement, two stimulation electrodes are positioned to target the specific area. This method helps limit the current flow primarily to the excitable tissue of interest.

Both poles (+) and (-) of each channel should be applied to the same muscle to be electrostimulated. Application of (+) and (-) electrostimulation channels on different muscles may result in lack of therapeutic effect due to improper stimulation, risk of burns on the patient, or potential risk of electric shock.

Do not exceed an intensity of 0.1 W/cm^2.
Follow these steps to ensure the reliability, safety, and accuracy of output parameters for your electrical stimulation.

13.3.1 EMS Programs - Electrode Arrangement


1. Ensure the electrical stimulation is turned off and Meissa OT LEDs do not indicate any abnormalities or program operation. before proceeding.
2. Select the size of the electrical stimulation electrode according to the width of the muscle being stimulated. Use larger electrodes for wider muscles and smaller electrodes for thinner muscles.
3. Connect the self-adhesive electrodes to the lead wire snaps of the same color.



4. Remove the protective liner from the electrode and save it for later use. Electrodes for electrostimulation are typically intended for multiple uses, so the liner will be needed to protect them between uses.
5. The skin must always be clean, dry, and free from lotion. Do not apply electrodes to injured skin.
6. Place the negative ("-") electrode on the proximal end of the muscle, securing it firmly to the skin. Apply the center first, then smooth down the edges of the electrode.
7. Place the positive ("+') electrode on the distal end of the same muscle. The distance between the electrodes should be at least 1 cm. Apply the center first, then smooth down the edges of the electrode.




13.3.2 EMG - Electrode Arrangement for EMG-triggered EMS Programs



Follow the chapter **13.3.1 EMS Programs - Electrode Arrangement**, to connect surface EMS electrodes (marked blue) to a single channel.

Place the third, reference EMS electrode (marked gray), connected to the white lead wire snap with "REF" label. The reference electrode must also be attached to the extremity undergoing therapy, positioned near a bony landmark.

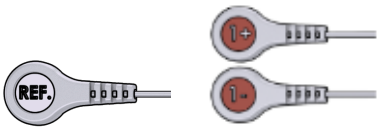

13.4 Electrical stimulation modes

The device allows the use of electrical stimulation according to pre-set programs. Details of the programs are described below.

Parameter	Description	Clinical relevance
Type of current	Direct current is, at most basic level, continuous and flows in only one direction. Alternating current passes first in one direction and then in another. Pulse current refers to either direct or alternating current in which there is a gap between successive pulses.	Direct current is used for iontophoresis. The alternating current is primarily used for innervated muscle contraction and sensory stimulation, with the pulses being continuous and combined. However, from the perspective of nerve excitation, the distinction between direct and alternating current is irrelevant. The pulse current differs from the alternating current because the pulses are separated. This separation means less energy may be delivered to the tissue when using this type of current.
Current amplitude	The magnitude of current is defined with reference to the zero-current baseline at a given moment. It can be referred to as the intensity of stimulation.	Increasing current amplitude will increase the energy delivered to the tissues under the electrode. This contributes to the sensory or motor response that the electrical current produces. The current amplitude is one of the determinants of torque production when using neuromuscular electrical stimulation. Increasing the current amplitude activates a higher percentage of muscle fibers; this results in a proportional increase in the torque produced and the size of the activated cross-sectional area of the stimulated muscle.
Current polarity	Biphasic pulse: charged particles move in one direction and then in the opposite direction.	If the current is polarized, physiological effects will include alterations in the cell membrane permeability, causing different responses under positive (anode) and negative (cathode) electrodes. For example, a marked hyperemia is usually expected under the cathode, while

Parameter	Description	Clinical relevance
		decreased nerve excitability is expected under the anode.
Pulse duration	The elapsed time between the beginning and end of all phases in a single pulse. It is often incorrectly labeled "pulse width" on a clinical stimulator.	The greater the pulse duration, the greater the skin impedance and the higher the patient's discomfort. Increasing pulse duration has been shown to enhance the charge of the pulse and increase motor unit recruitment. Alternating the pulse duration depends on the patient's comfort and the desired therapeutic effect. However, pulses with too short duration are inefficient.
Pulse frequency (f)	The number of pulse cycles generated per unit of time for pulse current.	The frequency of the pulses has been studied extensivecutly because of its important role in determining torque development and controlling muscle fatigue. Increasing frequency results in a sigmoidal increase in torque production, but it also accelerates muscle fatigue.
Waveform shape (shape rectangular)	The geometric shape of the pulse is represented on the graph of current (or voltage) versus time.	Limited clinical research has examined the effects of using different pulse shapes. Previous studies showed that there were individual differences in preferences for three different waveforms: sinusoidal, sawtooth, and square symmetric biphasic waveforms. There was no particular waveform identified as either the least or most comfortable for patients during neuromuscular electrical stimulation.
Stimulation mode (when more than one channel)	Reciprocal, asynchronous, or sequential.	Channels operate in a simultaneous or alternating fashion, according to a set duty cycle. In sequential stimulation, multiple stimulation channels are used (usually to activate multiple synergist muscles separately), allowing motor units to rest when the corresponding stimulation channel is not active. Asynchronous stimulation also utilizes multiple stimulation channels. However, the stimulus pulses are delivered in an interleaved manner, so that lower stimulation frequencies are achieved at each stimulation frequency is achieved at each stimulation channel while retaining a high composite stimulation frequency.

Medium-frequency alternating current parameters		
Carrier frequency	The frequency of the underlying alternating current waveform in the burst.	Medium frequencies are used to reduce the impedance of the skin and subcutaneous tissues, making the current more comfortable for the patient. Thus, by reducing skin impedance, the discomfort typically

Medium-frequency alternating current parameters		
		associated with traditional low-frequency current is minimized.
Burst	The generation of two or more consecutive pulse or cycles separated by a burst interval from the next series of consecutive pulse or cycles.	The burst duration plays a role in torque production, discomfort, and fatigue.
Burst frequency or modulation	The frequency at which bursts are generated.	This parameter influences the fatigue potential of muscles, particularly if the frequency is high (>50 or 60 Hz). At low frequencies (between 20 and 50 Hz), there is effective recruitment of nervous fibers, while at very low frequencies (2 to 10 Hz), the nervous fibers promote relaxation of the muscle fibers.
Burst duty cycle	The burst duty cycle of medium-frequency alternating current, expressed as a percentage, can be defined as the ratio of the burst duration to the total time of the cycle.	The burst duty cycle, similarly to burst duration, affects torque production, discomfort, and fatigue.

14. Notifications, Information, Errors, and Warnings displayed by the Software

The device also interacts with the user through errors, warnings, notifications and information displayed on the tablet. These notifications take the form of:


- dialog window,
- pop-up notification,
- configuration or exercise screens,
- inline text or checkmark notifications.

Meissa OT uses a color-coded system to indicate the type and severity of the notification:

- red is used for errors,
- yellow for warnings,
- and neutral (no color emphasis) for minor issues or informational messages,
- green for successful execution.

The following subsections of this chapter illustrate notifications and messages generated by the device, including errors and warnings along with their content and meaning.

14.1 Dialog window

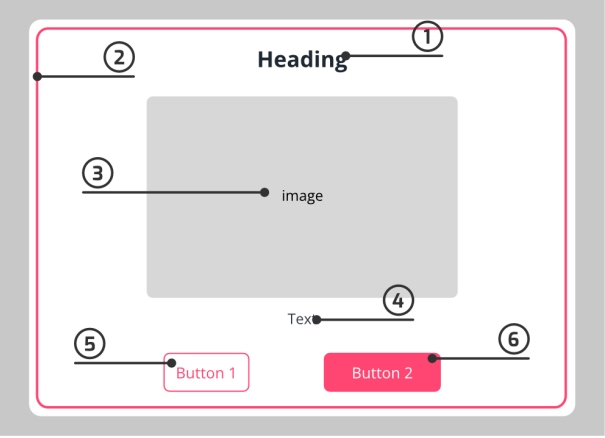

Dialog window - the general structure of dialog window.

The following table provides a description of the components used in the dialog window layout.

No.	Name	Operation description
1	Heading	Heading of alert modal (content).
2	Border	Border of the warning. The border color indicates the severity of the issue/information (as explained above).
3	Picture	Picture showing what is happening with the device.
4	Description	Text describing the situation and (if possible) how to solve it (meaning).

5	Sub button	Call an action (alternative option) - can be unavailable. The button color indicates the severity of the issue/information (as explained above). The button is styled as outlined.
6	Main button	Call an action (main option). The button color indicates the severity of the issue/information (as explained above). The button is styled as filled.

14.2 Pop-up notification



Example of a pop-up notification

14.3 Configuration or exercise screen



Example of a configuration/exercise screen


The following table provides a description of the typical components used in the configuration screen layout.



No.	Name	Operation description
1	Heading	Heading of the configuration screen (content)
2	Description	Text describing the information or the task to be performed (meaning)
3	Picture	Picture showing additional information to the description in field 2.
4	Next/Understand button	Confirms that the user has read and understood the displayed information or completed the action described in field 2. Pressing this button proceeds to the next step. The button may be disabled (grayed out) if certain conditions are not met – for example, if electrodes are not connected, are connected incorrectly, or if the appropriate device attachment has not been



		mounted. In such cases, the system prevents the user from continuing until the issue is resolved. Disabled Next button:  Yellow Next button:  If the displayed information includes a warning or requires special caution, the Next button is shown in yellow to highlight the increased level of attention needed before proceeding.
5	Back button	Returns the user to the previous step without confirming the information or completing the current action. This allows the user to review or modify the previous inputs before proceeding.


Additionally, configuration/exercise screens may include other elements (such as buttons, indicators, icons, etc.) that provide additional functions or information, such as those listed in the table below.

Picture	Name and description
	Step progress indicator - a visual element displayed on configuration screens to show the user's progress through a multi-step process. Each circle represents one screen or step. Circles are filled with a checkmark and turn green once the corresponding step has been completed. The current step is marked with a green outline, indicating the screen the user is currently viewing. This helps users track which screens they have already reviewed and how many steps remain.
	Additional button – provides an extra option apart from the standard Back and Next/I Understand buttons. This button typically allows the user to repeat an action that has already been performed.
	Settings/Configuration – opens the settings/configuration menu specific to the selected exercise type. This allows the user to adjust exercise-related parameters before starting the session. The available settings option depends on the chosen exercise type.

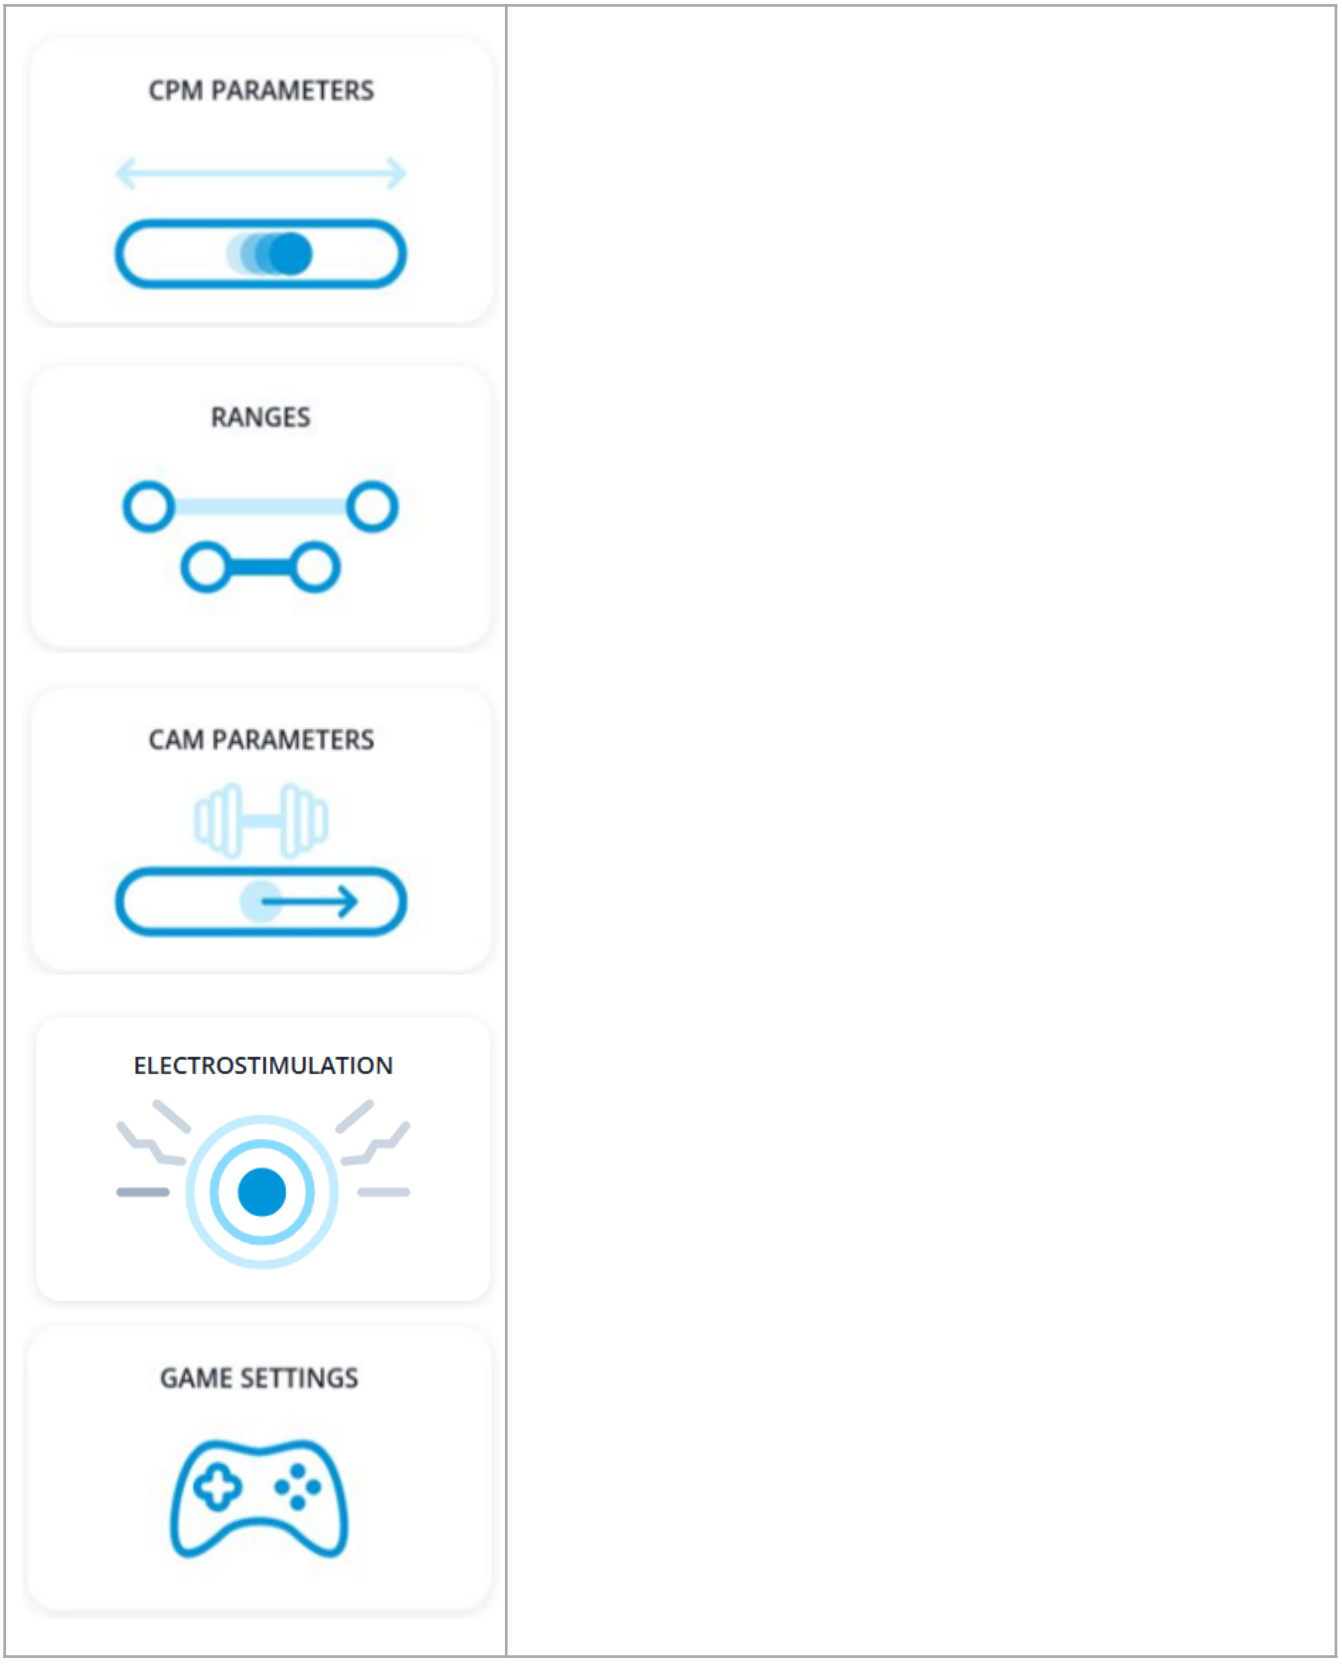

CPM PARAMETERS
RANGES
CAM PARAMETERS
ELECTROSTIMULATION
GAME SETTINGS

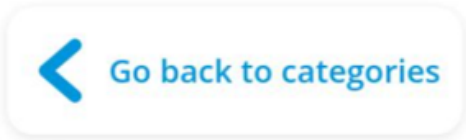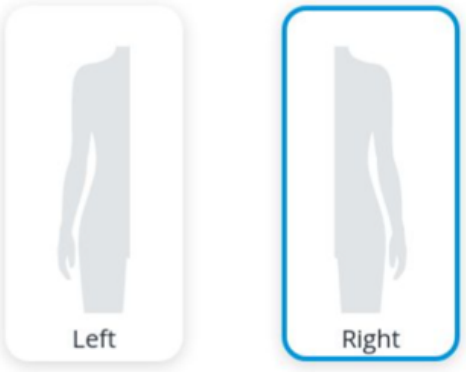
	Back to categories – returns the user to the list of setting/configuration categories, allowing them to select a different group of parameters or configuration options (e.g. CAM parameters, Game settings, etc.).
	+ / – – used to increase (+) or decrease (-) the value of a specific parameter. These buttons allow the user to adjust both numerical values and non-numerical settings, such as selecting between predefined options. Adjustments are made within defined limits or available choices. If the button is greyed out, it indicates that the current value or option cannot be changed further in that direction.
	Up / Down arrows – used to change the value of a specific parameter. These buttons allow the user to adjust selectable settings within defined limits/options. If the button is greyed out, it indicates that the current value or option cannot be changed further in that direction.
	Left / Right side selection – allows the user to choose which side of the body (left or right) will be exercised. The selected side is highlighted with a blue border, indicating the active choice.
	STOP – stops and locks the motor to hold the extension in the desired position during configuration, allowing safe placement of the patient's arm.
	Reset – restores the set range of motion to its default values. This function is available on the screen where the range of motion is configured and does not affect any other settings.

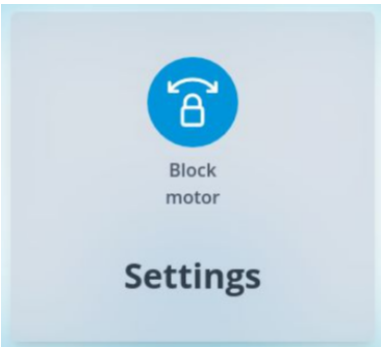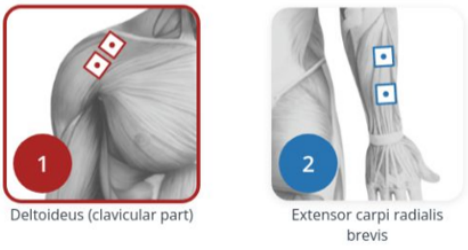	Screen button - the window appears after pressing the button below the device's screen. The block motor button allows users to block the motor on the screens where normally the extension socket is free to manoeuvre and unblock it on the screens where it is normally blocked.
	Muscle selection – allows the user to assign specific muscles to EMG/EMS channels. The border color and number shown on the selected muscle diagrams correspond to the color and number of the channel on the EMG/EMS cable. Muscles that have not been selected are displayed without a number and without a colored border, indicating no active channel assignment.
	Filtering and search fields – allow the user to narrow down the available options within the selected category. Filtering fields limit the displayed results based on predefined criteria, while the search field enables quick access by entering a keyword.
	Channel selection – allows the user to assign a function to one of the available, connected channels (e.g. triggering function). The selected channel is visually highlighted with a colored border, indicating it is currently chosen. Unselected connected channels are indicated by a colored number (matching the EMG/EMS channel) without a border.
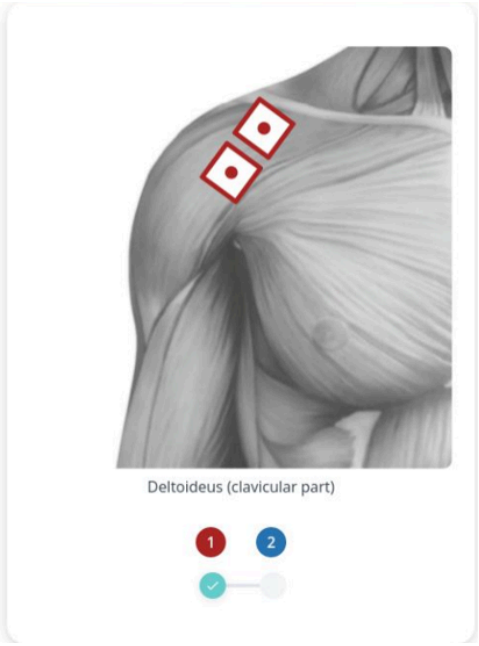
<table>
<tr>
<td> 
</td>
<td>Electrode connection confirmation – these indicators indicate the connection status of electrodes assigned to a specific EMG/EMS channel.

• A green checkmark confirms that the electrodes have been successfully and correctly connected.
• A gray circle indicates channels that have not yet been connected. These channels are pending setup and will be activated in sequence as the configuration progresses.
• An empty circle with a green outline marks the currently active channel, indicating that the user should now connect electrodes to this channel. The Next button will remain disabled (grayed out) until the channel is properly connected.
• An exclamation mark inside a yellow circle indicates poor signal quality on the connected electrodes. While the user is still allowed to proceed to the next step, the system draws attention to the suboptimal connection, which may affect signal accuracy. In this case, the Next button is also displayed in yellow with an exclamation mark, emphasizing the need for caution before continuing.
• An exclamation mark inside a red circle signals that the electrode has lost connection. In this case, the Next button is disabled (grayed out), and the user cannot proceed until the connection is re-established.</td>
</tr>
<tr>
<td> 
</td>
<td>Reset [label] – resets the recorded or set value (e.g., for torque, force, or MVC) associated with a specific function. In the case of MVC measurements, the button corresponds to the color of the channel from which the value was recorded. This allows the user to repeat the measurement and update the reference value.
The [label] may vary depending on the type of value being reset.</td>
</tr>
<tr>
<td>  </td>
<td>In-session settings – opens a menu with parameters that can be adjusted during the exercise session (incl. games).
In game modes, the button's visual style (e.g., color or shape details) may vary slightly, but it retains the gear icon shape.</td>
</tr>
</table>

	Stop – immediately stops the ongoing training session (incl. games). Once pressed, the session is permanently ended and cannot be resumed.
	Pause – temporarily stops the ongoing training session (incl. games), allowing it to be resumed from the same point without resetting progress and settings. In game modes, the button's visual style (e.g., color or shape details) may vary slightly, but it retains the two vertical bars shape (||).
	Play – resumes a previously paused training session (incl. games). In game modes, the button's visual style (e.g., color or shape details) may vary slightly, but it retains the triangular shape
	Finish – ends the training session.
	Show report – opens a report (summary) of the completed training session. The report details are described in chapter **14.8 Reports**.
	Download PDF - button to download the report as a PDF file to an external drive
	Stimulation channel selection – allows the user to select the EMG/EMS channel for which the electrical stimulation settings will be configured. The currently selected channel is highlighted in yellow, indicating that it is active for adjustment. The set stimulation value for the selected channel is displayed below the selection area.
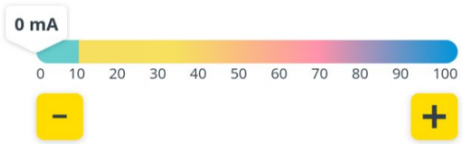
<table>
<tr>
<td> 
</td>
<td>Stimulation level slider – allows the user to adjust the intensity of electrical stimulation for the selected EMG/EMS channel. The slider is controlled by the + and – buttons; it cannot be adjusted by dragging. It visually represents the current stimulation range</td>
</tr>
<tr>
<td> 



Deltoideus (clavicular part)
 
Electrostimulation</td>
<td>Channel role assignment – Allows the user to assign a specific function to each EMG/EMS channel: either EMG trigger (EMG measurement) or electrical stimulation (EMS). This selection determines how the channel will operate during the session and defines the available configuration options.




 
Electrostimulation
Electrostimulation




 
EMG measurement
 
EMG measurement
EMG measurements only

 
Electrostimulation
+
Trigger
Trigger electrostimulation (EMG measurement) and to perform electrostimulation



 
EMG measurement
+
Trigger
Trigger electrostimulation and for EMG measurements</td>
</tr>
<tr>
<td>  </td>
<td>Exit menu – closes the current menu and returns to the training session.</td>
</tr>
</table>

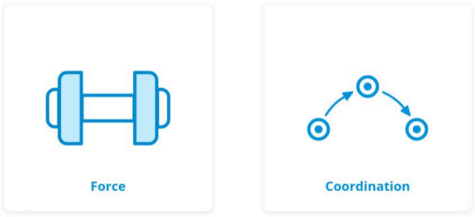
	Commit button – commits applied changes and returns to the exercise.
	Restore previous values – reverts the parameter settings to their previous state before any recent changes were made.
	Level type selection – allows the user to choose the type of exercise to be performed within the game environment: either force or coordination. This selection defines the gameplay logic. In the Force mode, the patient trains upper limb muscle force by moving along a track with a regular shape. In the Coordination mode, the patient navigates a more complex track, requiring dynamic changes in movement direction.
	Difficulty level selection – allows the user to choose the difficulty level of the game-based exercise. The estimated time required to complete the selected exercise is also displayed.
	Immediately stops the ongoing training session (games). Once pressed, the session is permanently ended and cannot be resumed. The user is redirected to the completed exercise screen, and session data is transmitted to the report.
	Mute – Turns off all in-game sounds. This does not affect system sounds, such as the audible notification associated with the emergency button, which remains active regardless of the mute setting.
	Add patient - opens the form for creating a new patient profile and adding them to the database.
	Patient Card - opens the patient card with access to their data and session history.

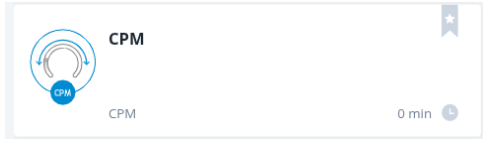	Start training - navigates to the training selection interface for the selected patient.
	Show report – displays the report of the selected completed training. The structure of the report is described in chapter **14.8 Reports**.
	Repeat training – restarts the selected training session using the previously configured parameters.
	Back - returns to the previous screen.
	My patients / All patients – switches the patient view mode between all registered patients and those assigned to the current user account.
	Favorite / All / Recent trainings – switches the training view between all available trainings, those marked as favorites, and recently performed sessions.
	Training tile – selects a specific type of training. Displays the training name, category, a bookmark icon to mark it as a favorite, and a clock icon with the duration time.
	Labeled input fields – used to enter specific information such as first name, last name, phone number, etc. Each field includes a title indicating the required data type and a placeholder text guiding the user on what to enter.

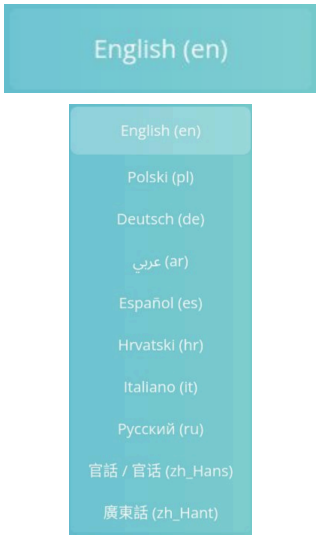
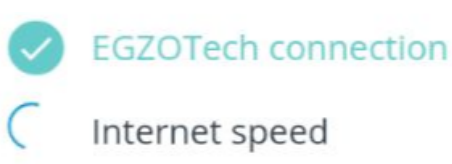
	Language change button - shows a list of all the available languages. Used to change the language of the application interface.
	User Manual button - lets users access the current User Manual from the application
	Help menu - button opens help menu
	WIFI button - informs if the device is connected to a WIFI network. Clicking it redirects to the WIFI connecting screen.
	Internet connection diagnostics - diagnoses the network's parameters.
	Diagnostics results - the spinning circle indicates that the diagnostics are in progress. The checkmark informs, that the module has been checked and works properly

Additionally, the software displays the information shown below.

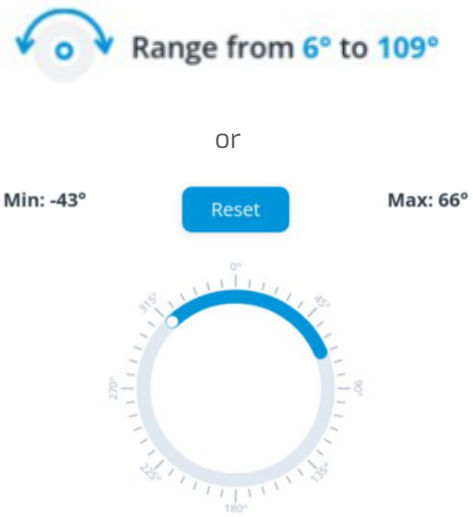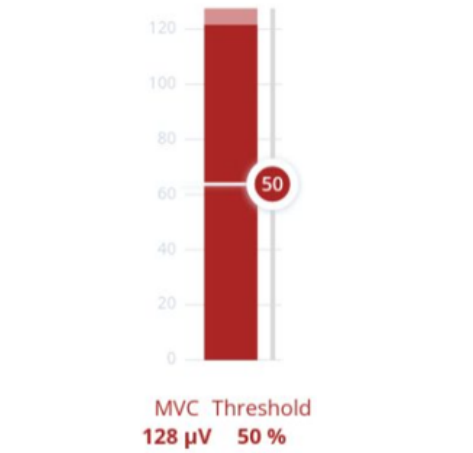
Picture	Name and description
	Indicates which side of the body (left or right) has been selected for the upcoming training session.
	Displays the configured starting and ending joint angles for the exercise as a blue arc, defining the total range in which the movement will occur. A white dot indicates the current position of the extension.
	Displays the user's measured maximum voluntary contraction (MVC) in microvolts and the configured threshold level (in percentage) required to trigger the movement. The red bar visualizes the threshold relative to the MVC value (current MVC relative to maximum recorded). The color of the bar and text corresponds to the EMG channel from which the signal is being measured and the threshold is applied.

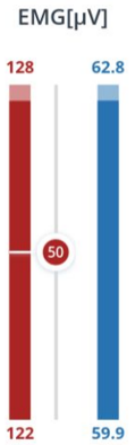	Displays the measured EMG activity (in microvolts) recorded from the assigned channels during EMG measurement (current MVC relative to maximum recorded). The bar's color corresponds to the EMG channel it represents. The values next to the bars indicate the current and maximum signal amplitudes. The numeric value displayed across one of the bars in a circle (e.g., "50"), indicates the configured threshold level, expressed as a percentage of the maximum voluntary contraction (MVC). This indicates the channel selected to trigger movement. The set threshold must be exceeded to initiate the movement.
	The software allows the training duration to be configured either by number of repetitions or by time. In repetition-based mode, the display shows the number of completed repetitions alongside the total number of planned repetitions. In time-based mode, a countdown timer indicates the remaining training time, and a separate counter displays the number of completed repetitions. Additionally, a progress bar is shown at the bottom of the screen, visualizing the user's progress. In repetition-based mode, the bar displays progress through the planned number of repetitions, along with the elapsed time.  In time-based mode, the bar represents the total exercise time, showing both elapsed and remaining time.
 and	The system displays the current joint position of the device's extension. This is shown in two forms: A 360-degree circular graph with a highlighted blue arc representing the configured range of motion for the exercise. A white dot moves along the circle to indicate the current position of the extension during movement. A numerical angle value is shown next to the graph, continuously updating to reflect the current position in degrees. The displayed value may be positive or negative, depending on the direction of movement relative to the 0° reference – positive for clockwise and negative for counterclockwise motion. The reference point 0° is located at the top center of the circle.

	
	PEC calibration PEC calibration result information - PEC calibration can be Required, Successful or Failed. PEC calibration result - informs users about the result of the PEC calibration. No action required. Calibrate button - starts the PEC calibration process.
	In game-based exercises, a time counter is displayed, showing the current time in minutes and seconds next to a clock icon. The color and style of both the counter and the clock symbol may vary depending on the game, however, it always appears as a clock icon accompanied by a numerical value.
	The point indicator shows the number of points earned during the game. The points serve purely as a motivational element for the patient. Points are awarded for staying within the required area and may be deducted when obstacles are encountered in some games. The color and style may vary depending on the game; however, it always appears as a star icon accompanied by a numerical value.
	The number of stars displayed at the end of the exercise reflects the player's performance, based on the number of points earned compared to the ideal game run (i.e., the player stayed within the designated path and avoided all obstacles). The number of stars serve purely as a motivational element for the patient. To earn stars depends on specific game and level. The maximum score is recorded either when the exercise is completed correctly or when the player exits the game using the "X" button. The maximum attainable score for a given session can be reviewed in the game report.
	The speed indicator appears in the Dream Drive game and represents the vehicle's current speed. Maximum speed is maintained during optimal performance, while deviations from the track or collisions result in reduced speed. The indicator serves as a motivational visual aid without functional impact on gameplay.

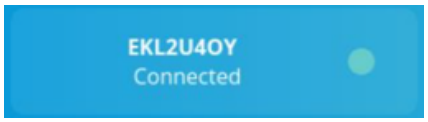	Informs the user on which floor they are currently on in the Elevator Express game.
 	Informs the user on which floor the character wants to step off the elevator in the Elevator Express game.
	Parkour Fever's control bars - arrows indicate which direction an user should move their limb to perform the next jump. Jumps are performed by sliding below the bottom line and then exceeding the top line. Repeat this sequence to perform the next jump.
	Jump trajectory in Parkour Fever - appears after exceeding the top line on the control bar and disappears after going below the top line, which is when the character jumps. Allows the user to determine where the character will jump.
	The software displays information about the serial number of the device and the connection status. “Connected” and green indicator indicates that the tablet is successfully communicating with the rest of the device components, including torque and force sensors, motors, and other subsystems.

14.4 Inline text or checkmark notification

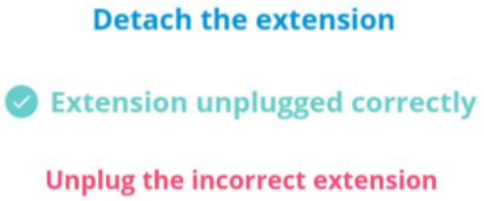

Inline text and checkmark notifications - the examples of the inline text or checkmark notifications


14.5 Errors

Please note that some messages may appear as errors, warnings, or notifications, depending on the stage of the session in which they occur. For example, disconnecting the extension during an exercise will be classified as an error, while the same event during the configuration phase will be displayed as an informational message.

Error list:

- "A communication error occurred with the device"
- "Missing Firmware Module"
- "Safety button pressed"
- "Detached cable"
- "Detached extension"
- "Spasticism has occurred"
- "Incorrect e-mail or password" - log in error
- "Please enter correct e-mail address" - log in error


The general structure of the error window is shown below.

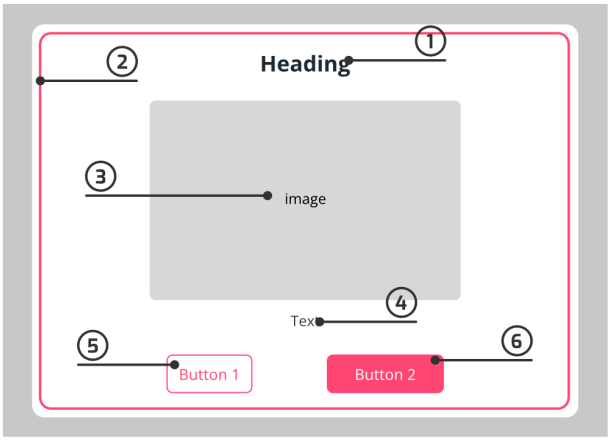


Error window - the general structure of the error window

14.6 Warnings

Examples of warning window structures are shown below.

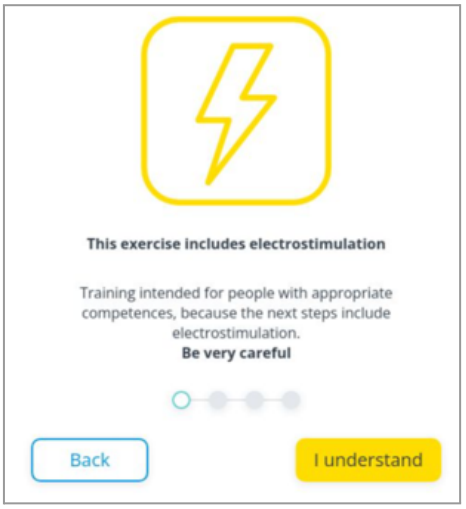

Warning window - the exemplary warning window

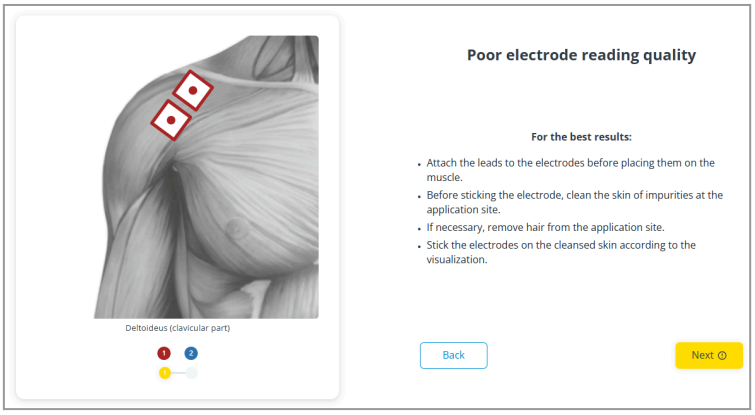


Warning window - the exemplary warning window

14.7 Notifications

Notification list:

- "Disconnected electrode"
- "Detached cable"
- "Detached extension"
- "Communication with the device has been successfully reset"

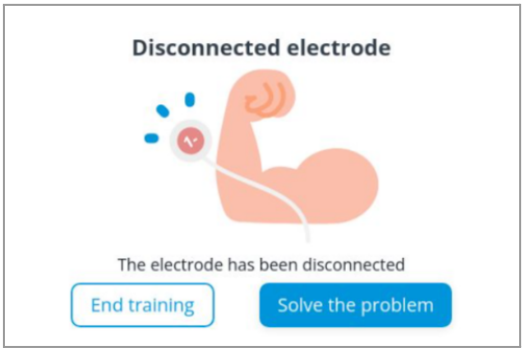


Notification window - the exemplary notification window

- “A new software version is available. Click here to update”




Pop-up notification - the exemplary pop-up notification

Configuration/ exercise notifications:

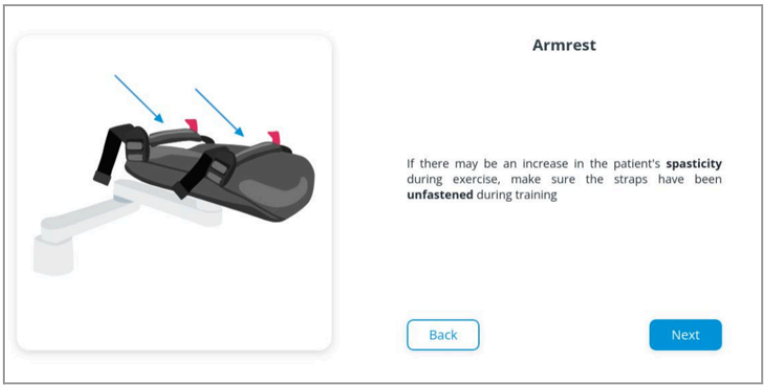

Configuration/exercise notification - the exemplary configuration/exercise notification

- “Do not use electrostimulation on the chest”
- “Do not use electrostimulation on the head”
- “It is forbidden to use electrostimulation near the neck and mouth”

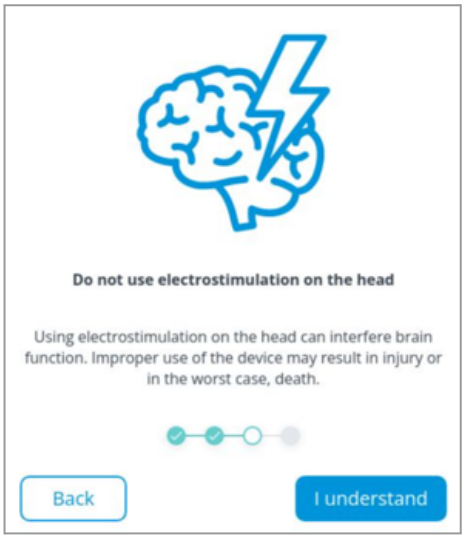

Configuration/exercise notification - the exemplary configuration/exercise notification


14.8 Reports

The software allows users to generate and view an exercise report after each completed session. **The report is intended for informational purposes only and should be interpreted exclusively by a qualified professional.**


The report provides a structured summary of the training and includes the following elements:

- Patient and specialist information (1),
- Session summary, including the date and time when the training session was performed, training type, total training time and number of completed repetitions (2),
    - The number of repetitions is displayed in red, yellow, or green, depending on how many were completed compared to the planned total. If **all planned repetitions** are completed, the number is shown in **green**. If **75% or more** (but not all) are completed, it is shown in **yellow**. If **less than 75%** are completed, the number is displayed in **red**.
- Exercise parameters, such as selected mode, repetitions, speed, pause time in ROM max/ROM min, movement direction, electrostimulation parameters (inc. no of phases, duration time, type, shape) (3),
- Basing data, including initial force calibration and range of motion values, exercised limb, and the exercised side of the body (4),
- Basic signal statistics showing minimum, maximum, average, and standard deviation for measured forces (5),
- Graphical extension's angle and signal waveforms representing real-time changes throughout the session (6),
- Exercise timeline with automatically logged events, such as pauses, resumed activity, and settings adjustments (7),
- Parameters for each EMG/EMS channel and selection of the applied function (EMG or EMS) (8).

The exemplary reports are shown below.

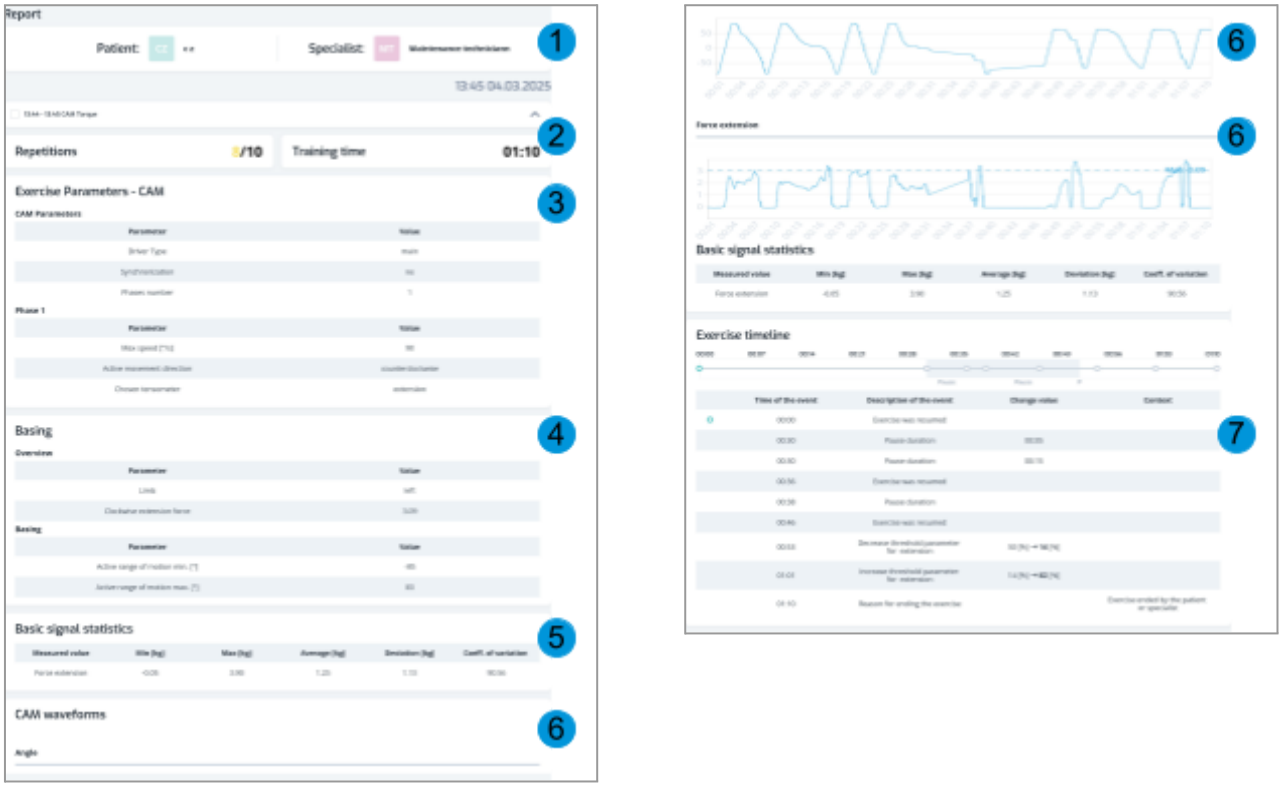

Example of a CAM Torque exercise report

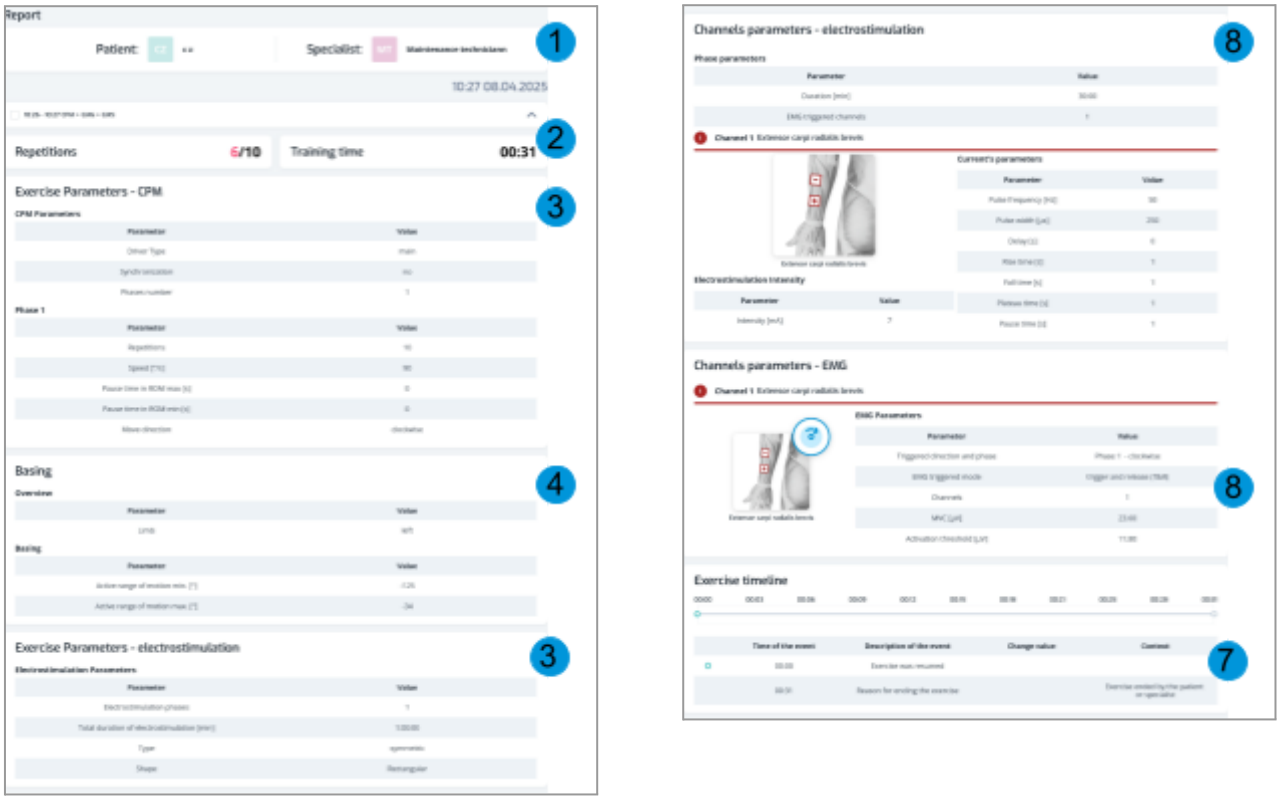


Example of a CPM + EMG + EMS exercise report


14.8.1 Saving a report to a USB drive

1. Connect the USB drive to the touchscreen display.


If the device does not detect the external USB drive the below window will appear.

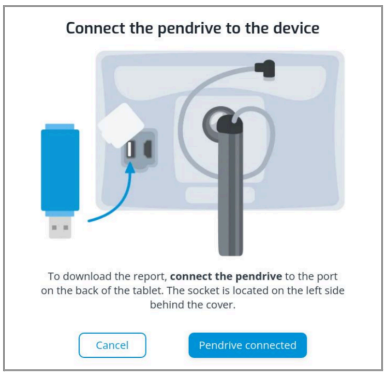


2. On the Patient card open the desired report.
3. Select the **Download Report** button.

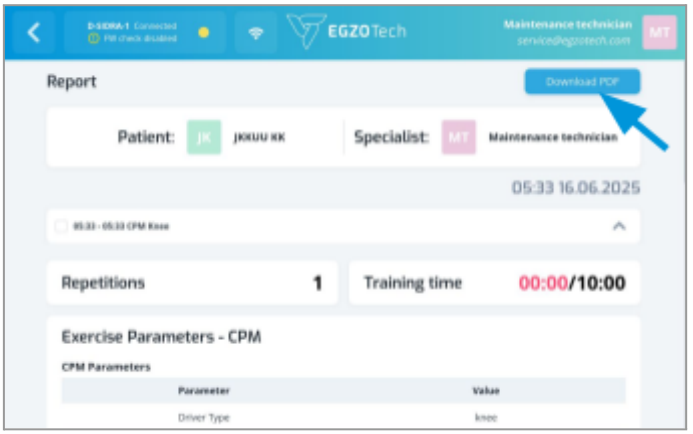

4. Wait until the download is complete.

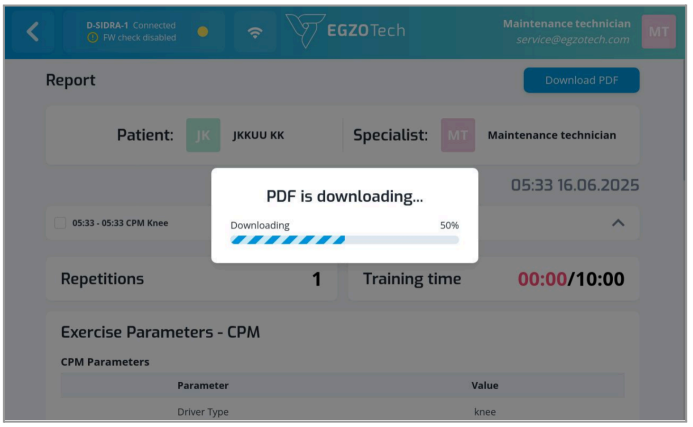

5. A confirmation message will indicate that the report was successfully downloaded.



15. Software

15.1 How to launch the application

Meissa OT's application is automatically launched on its tablet when the device AC cable is connected to the power supply source and power button is pressed.

15.2 Registration

The user creates a new clinic profile by filling out the registration form. Information such as the e-mail address, clinic name, user's name and surname is required. After registering the clinic, a password field will appear.

If your clinic profile already exists, refer to chapter **15.3 Signing in**.

15.3 Signing in

The user can sign in by entering their clinic's e-mail address and password on the application's home screen.

15.4 Clinic's profile

After logging in, the user will see a list of their patients.

15.5 Patient's profile

After clicking on the selected patient's tile, the therapist will see the patient's card, which includes the history of training sessions, clinical data, and training sessions prescribed by the therapist.

16. How to set up a training program

The following sequence of steps can be executed only after completing all the activities described in the chapter **2.3 Starting up your Meissa OT**.

Step 1: After selecting the patient, the user chooses an exercise they wish to perform from the training selection screen. The detailed training list is available in chapter **17. Programs Overview**. The training options are displayed in three categories: "Suggested," "Filters," and "All."

Step 2: Follow the instructions on the screen to continue with the Basing procedure.

Step 2.1: Choose the exercise parameters that suit the patient's needs, ensuring their safety and preventing any potential hazards.

Step 2.2: Select the trained side - left or right.

Step 2.3: Mount the required extension. If it has not been mounted yet, the application will notify you, and guide you through the extensions.

Step 2.4: Align the axis of the device with the correct one. Each axis of rotation is set independently. Ensure the patient is properly positioned during the exercise. It is recommended to perform the exercises in the anatomical position. For this reason, it is advisable to use a height-adjustable table.

Step 2.5: For every exercise, Basing will be required. The Basing consists of two stages:

- Measuring Passive Range of Motion (ROM): performed by Meissa OT during the maximal passive movement of the patient's hand using external assistance (clinician or therapist).
- Measuring Active Range of Motion (ROM) and Force: performed by Meissa OT during the active movement of the patient hand (without external assistance).

Step 3: (EMG/EMS in Meissa OT Ultra only) After choosing the training involving EMG or EMS, the user must perform the additional actions described below.


Step 3.1: (EMG/EMS in Meissa OT Ultra only) Connect the EMG cable using the socket located on the back of the chassis. The cable is correctly attached if you hear two "click" sounds, and it cannot be pulled off.

Step 3.2: (EMG/EMS in Meissa OT Ultra only) Select the patient's target muscles that need to be monitored or stimulated. The number of muscles that can be selected depends on the number of channels in the cable.
The channel colors in the software correspond to the lead wire colors.


Step 3.3: (EMG/EMS in Meissa OT Ultra only) Choose what function the channels will perform. In the EMG exercise, it can be a Triggering function. While in the EMS exercise, it can be Electrostimulation or Electromyography. In the EMS+EMG exercise, both functions are possible.

Step 3.4: **(EMG/EMS in Meissa OT Ultra only)**

Connect the electrodes to the appropriate lead wire channels before applying them to the patient's skin.
The user applies the electrodes to the patient's skin based on the electrode placement for the selected muscle or body part, as displayed in the software.
Choose the appropriate electrodes for the intended application - EMG electrodes for EMG Biofeedback and EMS electrodes for EMS program.
The user will see the electrode placement to guide them on how to place the electrodes correctly for that muscle.
Place the electrodes connected to the snaps with a "+" and "-" sign in the appropriate location, as shown in the icon.



Quadriceps femoris



If an exercise with elements of Electromyography was chosen, don't forget to connect the reference electrode to the white single lead wire (reference channel) marked with the REF sign if there is a gray electrode on the software icon.



Next to the channel icon is a marker indicating the quality of the connection between the electrode and the skin.
The channel colors in the software correspond to the lead wire colors.
When all electrodes are successfully connected, you can proceed.
For more detailed instructions on electrode choice and electrode placement see chapter **13.3 EMS Electrode arrangement and configurations** and chapter **12.4 EMG Electrode arrangement and configurations**.



Use only electrodes authorized by **EGZO**Tech, as described in chapters **9.3 Electrodes for surface electromyography** and **9.4 Electrodes for electrostimulation**. **Electrodes of inadequate size or unsuitable application could provoke skin reactions or burns**. Electrode properties such as dimensions, conductivity, impedance, and connector types can greatly influence safety. **Never use ECG/EMG electrodes for the purpose of electrical stimulation**.

Step 3.5: **(EMG/EMS in Meissa OT Ultra only)**

In the EMG-triggered programs, it is necessary to calibrate the measurement range. To do this, generate a Maximal Voluntary Contraction (MVC) with the muscle(s) on which the electrodes are located, then set the threshold for the triggering channel. You can also change the threshold during the exercise later.
In programs that use electrostimulation, it is also necessary to calibrate the intensity of the flowing current according to the individual patient's comfort level before starting the workout. Press "+1" to increase the intensity and "-1" to decrease the intensity by 1 mA. This can be recalibrated later during the exercise.

In the EMG+EMS exercise, both steps need to be completed.
Once the setup is done, press the “Next” button.

Step 3.6: (EMG/EMS in Meissa OT Ultra only) If the exercises CAM Isokinetic, CAM Isokinetic Turn Key, or CPM+Force were chosen, the Maximum Force needs to be measured, and the threshold should be set. You can also change the threshold during the exercise later.

Step 4: The user confirms being readiness to start the training.

Step 5: To begin the training, press the “Play” button. Treatment display views vary for the different exercises.
Some parameters can be reset during the exercise, after clicking the gear icon.

Step 6: After training is complete, an autogenerated report can be viewed. If electrodes were used during training, they should now be disconnected from the patient.

Step 7: Check and follow the instructions in chapters **2.5 Finishing your work with Meissa OT** and **19. Cleaning**.

16.1 What exercises can I perform?

All training modes are described in chapter **17. Programs Overview**.



Meissa OT is constantly evolving. Therefore, we’ve provided you with the most recent exercise manual in the package. However, be sure to check our website http://courses.egzotech.com and the application notifications after each update to find out the newest exercises added to your machine.

17. Programs Overview

Meissa OT device is controlled using the touchscreen equipped with proper software - EGZOClinic. Although the software operates fully offline on each device using a dedicated local database, an internet connection is required to receive updates.

The software offers different type of programs and functions, mainly:

- Continuous Passive Motion (CPM)
    - CPM
    - CPM Force
    - CPM + EMS (Meissa OT Ultra only)
    - CPM + EMG (Meissa OT Ultra only)
    - CPM + EMG + EMS (Meissa OT Ultra only)
- Continuous Active Motion (CAM)
    - CAM Isokinetic
    - CAM Torque
    - CAM Turn Key
    - CAM Games (Cosmic Mission, Dream Drive, Ocean Paradise, Cat Crunch, Doggo Nom, Rope-Nope, Elevator Express, Parkour Fever)
- Electrostimulation programs (EMS) (Meissa OT Ultra only)
- Electromyography programs (EMG) (Meissa OT Ultra only).

17.1 Continuous Passive Motion (CPM)

17.1.1 CPM

Regular Continuous Passive Motion (CPM) is a standard therapy exercise where Meissa OT applies a set torque, moving a static patient through the specified range of motion at a set maximum speed. When a maximum value of the range of motion is reached, CPM will switch the direction of the applied torque and guide the patient's limb in the opposite direction. During the CPM, the patient is to remain static.

17.1.2 CPM Force

Continuous passive movement is triggered by the patient's muscle strength. During calibration, the patient applies pressure on the extension (for the "drive" option, it can be any extension, for the "extension" option, the "key" extension should be used). The force level is selected for the chosen direction, or, in the case of bidirectional movement, for both directions. Then, during the exercise, the patient must generate pressure above the threshold selected by the therapist. When this is done, the extension moves the patient's hand to the end of the set range of motion. If it is a movement in one direction, the extension will return passively to the initial position; if bidirectional, the patient must again generate pressure above the threshold.

17.1.3 CPM + EMS (Meissa OT Ultra only)

Continuous Passive Movement with synchronized electrostimulation of the selected muscle involves moving the patient's hand from one end of the range of motion to the other at a set maximum speed. The electrostimulation is activated during one of the selected movement phases. The patient remains passive during the exercise. The electrostimulation supports neuromuscular activation and re-education.

17.1.4 CPM + EMG (Meissa OT Ultra only)

Continuous Passive Movement triggered by the patient's muscle activity by EMG. During calibration, the activity of the selected muscle using EMG is collected and the threshold is selected. Then, after starting the exercise,

the patient must, depending on the selected mode (trigger & release or trigger & hold), generate muscle activity above the threshold or generate and maintain it throughout the entire range of movement performed by the robot.

17.1.5 CPM + EMG + EMS (Meissa OT Ultra only)

Continuous Passive Movement with electrostimulation triggered by the patient's muscle activity. During calibration, the activity of the selected muscle using EMG is collected and the threshold is selected. Then, after starting the exercise, the patient must, depending on the selected mode (trigger & release or trigger & hold), generate muscle activity above the threshold or generate and maintain it throughout the entire range of movement performed by the robot. Electrostimulation is triggered simultaneously with the selected direction of movement.

17.2 Continuous Active Motion (CAM)

17.2.1 CAM Isokinetic

Continuous Active Motion (CAM) consists of exercises where Meissa OT provides dynamic resistance (based on the applied torque) and allows the patient to move freely throughout the range of motion. The movement speed is constant during the whole movement (after exceeding the threshold). Dynamic reversal is achieved when the patient voluntarily participates in dynamically and rapidly changing the direction of movement upon reaching the end of the range of motion. With such exercises, an evaluation of the maximal muscle strength can be performed.

17.2.2 CAM Torque


CAM Torque consists of exercises where Meissa OT provides dynamic resistance based on the applied torque, allowing the patient to move freely throughout the range of motion. The movement speed is proportional to the applied force — after exceeding the threshold, the device moves slowly at first and accelerates as the force increases. Dynamic reversal is achieved when the patient voluntarily and rapidly changes the direction of movement upon reaching the end of the range of motion. With such exercises, an evaluation of maximal muscle strength can be performed.

17.2.3 CAM Turn Key

CAM Turn Key is a type of Continuous Active Motion exercise in which the patient turns an extension called the Pinch meter, imitating the motion of turning a key in a lock. To rotate the extension, the set thresholds for both pinch force and rotation force must be exceeded simultaneously. Upon reaching the end of the range of motion, the patient can either turn the extension in the opposite direction while maintaining the same principles or allow it to return automatically, depending on the selected setting.

17.2.4 CAM Games

Before selected games, a simple tutorial is displayed in the software to explain how the game works. It provides a clear visual guide to the game mechanics, helping the user understand how to interact with the game effectively.

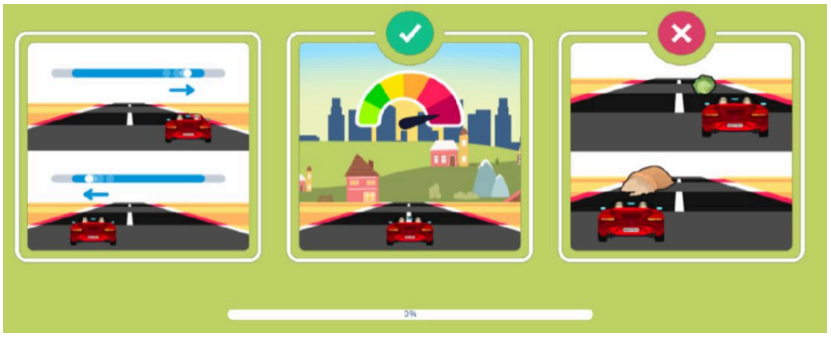

Example of game tutorial for Dream Drive game

17.2.4.1 CAM Game "Cosmic Mission"

A game in which the patient's task is to move the extension along a designated path within the range of motion selected during configuration (turning to the right raises the ship, while turning to the left lowers it). The game offers two types of exercises: Strength and Coordination. In the "Strength" module, the patient works on the strength of the upper limb muscles by moving along a track of a regular shape. In the "Coordination" module, the patient must dynamically change the direction of movement by navigating along a more complicated track. Each module is divided into several difficulty levels. The extension moves as it does in the Isokinetic CAM Classic exercise.

17.2.4.2 CAM Game "Dream Drive"

A game in which the player controls a car using a special adapter. The goal is to cover the longest possible distance within a set time. The car moves faster when it stays on the road, but if it goes off-track, it slows down. Obstacles appear along the route, which must be avoided to maintain speed.

The game offers two gameplay modes: strength and coordination. The strength mode involves navigating a track with many turns, requiring intense muscle work and increased endurance. The player must maintain stable control of the vehicle despite dynamic direction changes. The coordination mode focuses on precise vehicle control. The track is designed to develop movement control and the ability to react quickly to changing conditions.

The player can adjust the difficulty level by modifying the vehicle's speed and the frequency of obstacles. This allows the game to be tailored to the user's individual needs.

Each mode is divided into several difficulty levels. The adapter moves according to the principles of the Isokinetic CAM Classic exercise.

17.2.4.3 CAM Game "Ocean Paradise"

The player controls a sea turtle in a simulated aquatic environment, tasked with collecting a specified number of coins within a set time limit. During gameplay, they must avoid interactions with a paparazzi diver, which hinders movement and optimization of the movement trajectory.

The game mechanics feature a power-up system that allows temporary modulation of control parameters. The player can access bonuses such as a protective shield against the diver's negative influence, a x2 multiplier for collected coins, a magnet that automatically attracts coins, and an extra life.

Gameplay is divided into two modes: strength and coordination. The strength mode emphasizes movement intensity and frequency, requiring increased activation of muscle groups. The coin layout is designed to enforce repetitive, controlled movements that support endurance development and motor stabilization. The coordination mode focuses on precise control and adaptation to dynamic environmental changes. The coin

positions are arranged to require high accuracy in movement trajectory, aiding in proprioception and manual control development.

The player can adjust the difficulty level by selecting parameters that affect the game's dynamics. The adapter operates according to the biomechanical principles of the Isokinetic CAM Classic system, ensuring realistic motion replication in a controlled environment.

17.2.4.4 CAM Game "Cat Crunch"

A game in which the patient's task is to control a cat moving left and right within a predetermined range of motion, aiming to catch falling fish while avoiding harmful objects such as cans. The game offers two gameplay modes: Score and Goal. In the "Score" mode, the objective is to achieve the highest possible score within a set time limit. In the "Goal" mode, the patient must collect a specific number of fish while maintaining their lives. Hearts occasionally appear to restore lost lives, up to a maximum of three. The game includes four difficulty settings that adjust the speed of falling objects and the frequency of cans, progressively increasing the challenge across eight levels. The device moves in accordance with the principles of the Isokinetic CAM Isokinetic exercise.

17.2.4.5 CAM Game "Doggo Nom"

A game in which the patient's task is to guide a dog moving sideways within a predefined range of motion, catching falling dog treats while avoiding obstacles such as lemons. The game offers two gameplay modes: Score and Goal. In the "Score" mode, the objective is to achieve the highest possible score within a set time limit. In the "Goal" mode, the patient must collect a specific number of fish while maintaining their lives. Hearts occasionally appear to restore lost lives, up to a maximum of three. The game includes four difficulty settings that adjust the speed of falling objects and the frequency of cans, progressively increasing the challenge across eight levels. The device moves in accordance with the principles of the Isokinetic CAM Isokinetic exercise.

17.2.4.6 CAM Game "Rope-Nope"

A game in which the patient controls rotating swords of different colors, aiming to cut falling ropes that match the color of the active sword. Each rope can only be cut by the sword of the corresponding color — for example, the red sword cuts red ropes, and the blue sword cuts blue ropes. The game features two modes: one where the goal is to cut a specific number of ropes, and another where the patient aims for the highest score within a time limit. There are four difficulty levels that adjust the speed and frequency of the falling ropes.

Players start with three lives. A life is lost if the wrong sword is used to cut a rope. However, lives can be regained by cutting 10 ropes consecutively without mistakes. Additionally, every five successful cuts trigger a combo, multiplying the score but also accelerating the rope speed, which increases the overall challenge. The game consists of 8 levels, each progressively harder.

The device moves according to the principles of the Isokinetic CAM Isokinetic exercise.

17.2.4.7 CAM Game "Elevator Express"

A game in which the patient controls an elevator moving up and down to transport the guests to the right floors, earning a point for every successful arrival, and losing one point for stopping at a wrong level. There is one mode - a time-based score challenge, where the goal is to gain as many points as possible in the given time. The game has four difficulty levels that increase the number of floors. The game features 4 levels that get progressively harder.

The device moves according to the principles of the Isokinetic CAM Isokinetic exercise.

17.2.4.8 CAM Game "Parkour Fever"

A game where the patient controls a mage. The creature is moving right and left on its own. The control bar is located on the left side of the screen. While exceeding the upper line on the bar the jump trajectory appears, and the mage jumps after moving the limb to a position under the upper line. To jump again the device's position firstly must be below the bottom line. The target is to go higher and higher to collect all shiny orbs located on various platforms.

There is one mode - a time-based score challenge, where the goal is to gain as many points as possible in the given time. The game has four difficulty levels that increase the number of special platforms. The game features 4 levels that get progressively harder.

The device moves according to the principles of the Isokinetic CAM Isokinetic exercise.

17.3 EMS Programs settings (Meissa OT Ultra only)

In the following subchapters, you will find possible settings for typical electrical stimulation procedures. They are valid for the load impedances specified in section 10.2 Technical Specifications.

17.3.1 EMS programs details

EMS programs details	
Type of current	Biphasic symmetric
Shape	Rectangular
Repetitions	5 - 100
ROM max (deg)	Max passive ROM
ROM min (deg)	Min passive ROM
Starting point	Max / min
Move direction	Clockwise (starting point in min) / Counterclockwise (starting point in max)
Pause time in ROM max (s)	0 - 60
Pause time in ROM min (s)	0 - 60
Channels min	1
Channels max	4
Frequency (Hz)	5/10/15/20/25/30/35/40/45/50/60/70/80/90/100
Pulse duration (µs)	50/100/150/.../500
Pulse rise time (s)	0/1/2/3/4
Pulse plateau time (s)	1/2/3/.../20
Pulse fall time (s)	0/1/2/3/4

Meissa OT Ultra provides the following programs involving electrostimulation:

- Continuous Passive Motion (CPM) + EMS,
- Continuous Passive Motion (CPM) + EMG + EMS.

Depending on the desired effect of electrostimulation on a patient's muscles, one of the following four frequency ranges can be chosen for each type of program involving EMS offered by Meissa OT Ultra medical device.

Frequency (Hz)	Effect on muscle
1 - 10	Generation of a single contraction. Activation of slow-contracting, fatigue-resistant muscle fibers.
10 - 20	Partial muscle contraction. Increasing the muscle's endurance.
20 - 50	Tetanic contraction. Activation of fast muscle fibers. Increase in muscle strength.
69 - 90	Increasingly stronger tetanic contraction. Increase in muscle strength and muscle mass.

17.3.2 Custom EMS Program settings

All of the possible input parameters and ranges for the custom electrostimulation program have been listed below.

Input parameters of Custom EMS program	
Duration (repetitions)	5/10/15/20/50/100
Intensity (mA)	0 - 99
Pulse duration (µs)	50/100/150/.../500
Frequency (Hz)	5/10/15/20/25/30/35/40/45/50/60/70/80/90/100
Rise time (s)	0/1/2/3/4
Fall time (s)	0/1/2/3/4
Plateau time (s)	1/2/3/.../20

17.4 Typical use cases

The schemes of device use were defined on the basis of a device usability analysis.

Use by a Professional User

1. The therapist turns on the device by pressing the Power Button on its cover.
2. The therapist signing up/logging in to the Clinic,
3. The therapist chooses the patient's profile or creates a new one.
4. The therapist places the appropriate extension in the device.

5. The therapist chooses an exercise for the patient.
6. The therapist connects electrodes to the patient (Meissa OT Ultra only).
7. The patient performs the training.
8. The therapist can view an auto-generated training report after finishing the training.
9. The therapist unfastens the patient from the device and electrodes (if used).
10. After finishing the training, the therapist turns off the device and cleans it.

Use by a Lay Person


1. The healthcare professional has prescripted exercises on Meissa OT.
2. The operator turns on the device by pressing the Power Button on its cover.
3. The operator signing up/logging in.
4. The operator chooses the patient's profile or creates a new one.
5. The operator places the appropriate extension in the device.
6. The operator chooses the prescripted exercise from a list of exercises.
7. The operator connects electrodes to the patient (Meissa OT Ultra only).
8. The patient performs the exercises.
9. After finishing the training, the operator turns off the device and cleans it.

18. Miscellaneous


18.1 How to identify your Meissa OT or accessories

When troubleshooting and consulting with your product specialist or customer support, you may be asked to provide your Meissa OT Serial Number or the Serial Number of your accessories (inc. extensions).

Meissa OT serial number can be found on a label located at the back of the platform, which looks like this:

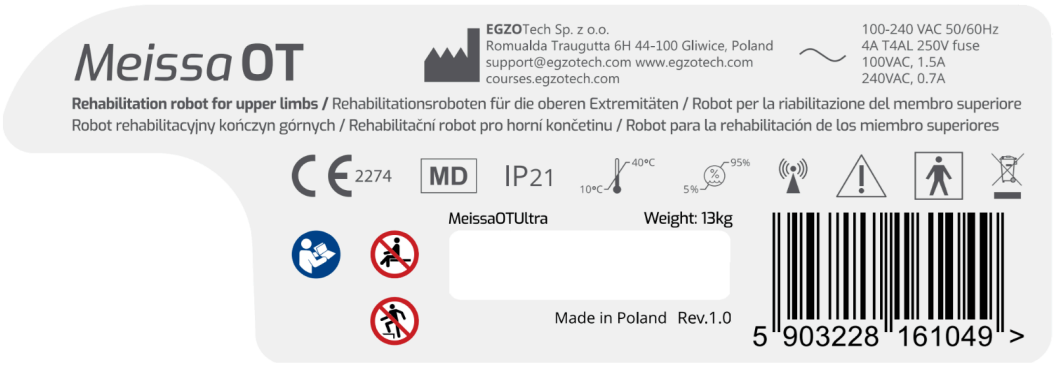


or

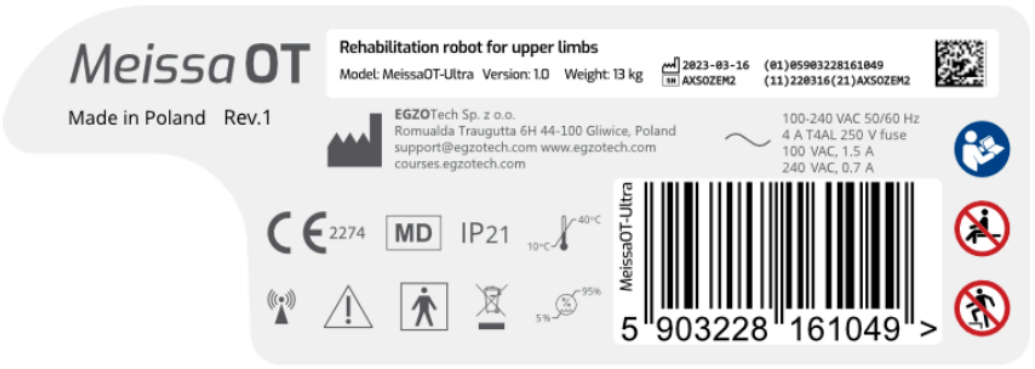

Due to the ongoing transitional period, the device may be supplied with one of the labeling versions listed above. The specific label applied depends on the device model and production batch.

In the white box on the label located on the left side of DataMatrix, you can find the serial number (SN).
All extensions have similar labels as shown in the example below. Always check the serial number (SN) when referencing accessories.

Label of Meissa OT accessories:

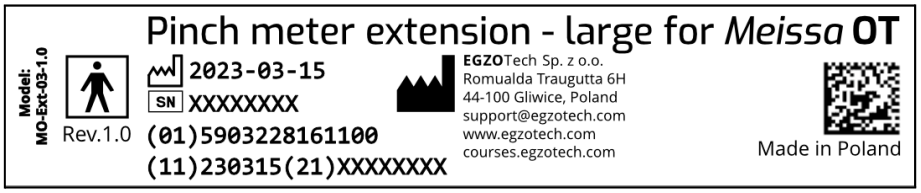

18.2 Behaviour of Meissa OT

Meissa OT device emits only one visual (light) informative notification when powered on, as indicated in the table below. Refer to chapter **10.6 LED Ring - Visual notification** for more information.

Status	Action by Operator	Description
Power OFF	Power OFF Meissa OT	The LED ring is not lit
Power ON	Power ON Meissa OT	The LED Ring lights up in blue, with a green point indicating the extension's position*.

* The exact position of the extension is provided within the software, which displays this information. Therefore, the green point serves primarily a decorative or supportive function rather than providing essential information for the user.

18.3 Description of user maintenance responsibility

The consumable items for Meissa OT:

- EMG electrodes - Designed for single use (Meissa OT Ultra only),
- Electrical stimulation electrodes - Designed for single-person use only. Note: The lifetime of the electrode varies depending on skin conditions, skin preparation, type of stimulation, storage and climate (Meissa OT Ultra only),

The user is obliged to report the need for annual inspections.

It is suggested to regularly restock your supply to ensure availability when needed.

18.4 Software auto updates

Meissa OT will occasionally want to perform software auto updates for both the tablet application and electronic modules. You will be notified of these updates through a popup window. Software updates ensure that Meissa OT remains safe and may include enhancements in exercises, games, manuals etc.



Because software updates include safety enhancements, allow Meissa OT to update as notifications arrive.

Ensure that Meissa OT's range of motion is not restricted by any external objects, yourself, or your patients.

The **maintenance visits** for Meissa OT **should be performed not less frequently than once a year**.

18.5 Electrical isolation information

This chapter provides basic information on how AC voltage is isolated in Meissa OT:

- Meissa OT is equipped with an integrated fuse AC power supply socket type C14 according to IEC 60320 to connect the power cord described in chapter **9.1.2 AC Power Cable**.
- In a professional healthcare environment, to completely disconnect the device from the electrical power supply, unplug the mains cable or set the mains switch to the OFF position.
- For home healthcare environment equipment disconnecting the AC cable is not permitted for the user. Detaching the cable from the connector of the device is allowed only by authorised service of the manufacturer equipped with a dedicated disconnection tool.
- Disconnecting the AC cable or turning OFF the switch disconnects both poles of AC voltage power.
- The use of the emergency stop push buttons described in chapter **10.9 Emergency stop push buttons**, disconnects only 24 V internal power supply circuits. The AC power supply circuits remain connected after using the emergency stop push buttons.

- All voltages above 60 V DC or 42.4 V AC inside Meissa OT's chassis that cannot be disabled by the AC power switch are additionally protected and isolated. A BF applied symbol (a patient inside the square) is located on the product label described in chapter **18.1 How to identify your Meissa OT or extensions?**

18.6 Expected product service life

The expected product service life of Meissa OT is 5 years, under normal operating conditions and receives proper maintenance and handling. The accessories and detachable parts of Meissa OT **will experience normal wear and tear**, which will decrease the overall product service life.

The expected shelf life and service life for accessories, including surface components, may differ. Please refer to their associated documents and packaging for more information. Do not use them after the use-by date.

If you notice any decline in performance of Meissa OT's parts, particularly the chassis or any of the accessories, please consider replacing them.

Due to the moving mechanical parts, Meissa OT will experience wear and tear. Given that some safety features rely on these mechanical components, periodic maintenance is required based on your Meissa OT usage. With the implementation of two patient protection methods for mechanical hazards, maintenance can be performed after a single fault occurs. Official maintenance personnel approved by **EGZO**Tech or its partners can conduct periodic maintenance to ensure the device's continuous stability and reliability and to prevent single fault conditions. If your Meissa OT has a stable, unrestricted Internet connection available at all times, your usage will be monitored by **EGZO**Tech and its partners.

18.7 Storage and transportation instructions

The device and accessories should be stored and transported in its case, however for internal transport it is permissible to move Meissa OT unboxed in its transport position within one building.

Before transporting the device, turn off the main power button and disconnect Meissa OT from the power source by unplugging the AC cable or using the installation disconnector (for home healthcare environment equipment disconnecting the AC cable is not permitted for the user. Detaching the cable from the connector of the device is allowed only by authorised service of the manufacturer equipped with a dedicated disconnection tool).

A safe transport position for the device is shown below. In this position the device should be moved from place to place and placed in its packaging.





The head of the device is turned to the side and is locked, the tablet holder is folded - the safety band is attached to the tablet holder, take care that the tablet holder does not make uncontrolled movements when being carried causing a risk of collision, the tablet is rotated. Take care when moving to avoid collision with any other object.



Beware of the risk of dropping the device during transportation. **In the event of dropping, the device must not be used** until it has been repaired, fully functionally tested and safety tested by an authorised manufacturer's service personnel.

Please mind that the underestimation of the device's weight, details in **10.2 Technical Specifications** may lead to handling difficulty.

Carefully place the device in its transport position in its case according to the cut-out at the bottom of the packaging. Place the device inside its packaging, placing the extensions in a way that matches the shapes of the cut-outs in the foam filling the packaging.

The device must be kept in a dry environment and should not be immersed in water or any liquid.

The storage and transportation conditions for Meissa OT should be:

- Temperature: 10°C to 40°C.
- Relative humidity: 10% to 95% RH, non-condensing.

Do not expose Meissa OT and its accessories to temperatures and humidity exceeding the specified range. To prevent short circuits, which can pose burn hazards or lead to gas release, do not store metal jewelry, metal-covered tables, or metal belts alongside the device.

Always check the special storage and usage conditions of the device and accessories specified on their labels, packaging and accompanying documentation.

The operator should check with the carrier to confirm how the device can be carried on the airplane.

18.8 How to safely dispose of the device

Meissa OT contains electrical and electronic components that may include materials harmful to the environment if disposed of with general waste. Residents of the European Union must follow specific disposal or recycling instructions for this product. While residents outside the EU should dispose of or recycle it in accordance with applicable local laws and regulations.



The symbol indicates that the product should not be discarded as unsorted waste but must be sent to designated collection facilities for recovery and recycling according to local regulations.

The equipment must be delivered to a suitable collection point for the treatment. By doing so, you contribute to the conservation of natural resources and the protection of human health.

Electrodes should be disposed of according to the instructions provided in their package.

18.9 Warranty

EGZOTech Sp. z o.o. provides a warranty to the original purchaser for this product for a period of 1 year from the date of purchase.

During the warranty period, the manufacturer will replace your faulty Meissa OT or accessories at no charge (except shipping and handling fees in some cases), provided that the product:

- Has been used for the intended purpose and in the manner described in this manual.
- Has not been connected to an unsuitable power source.
- Has not been subjected to misuse or neglect.
- Has not been modified or repaired.
- Has not been damaged further by shock.

Legal rights are not affected by this warranty.

Warranty conditions are detailed in the EULA. Before accepting the terms, please carefully read the content available at the website: https://support.egzotech.com/terms-and-conditions.

18.10 Manufacturer's service obligation

EGZOTech Sp. z o.o. provides the option to share, on demand, electrical schematic, bill of materials, descriptions, calibration manuals, and other information useful for authorized service personnel necessary for the repair of serviceable parts permitted by the manufacturer.

19. Cleaning

For long life and excellent quality, remember to clean Meissa OT, extensions and accessories regularly. Follow the guidelines below:

Meissa OT, accessories and components	Process Instructions
The device components and accessories: • base with head and table clamp, • tablet screen, housing and holder, • Extensions, • Arm Support set, • Electric Table with control panel, • fabric-based accessories: straps, belts and cushions, • EMG/EMS cable, • AC cables. Types of material used: • plastics, • metal, • fabric, • rubber (neopren), • laminated wood.	**STEP 1: Preparation before cleaning** **Preparation equipment:** A. Disposable protective gloves for the cleaning operative. **Preparation process:** A. Turn off the main power button. B. Disconnect Meissa OT from the power source by unplugging the AC cable (professional use) or disconnect the mains power of the device from the power supply using the fuse switch disconnector (home healthcare environment). **Note**: Remember that disconnecting the AC cable in home healthcare environment by the user is not permitted. C. Remove the extension and disconnect the EMG/EMS cable. D. Detach Meissa OT from Table clamp. E. Remove Meissa OT from Electric Table or other table on which it is mounted. F. Detach Arm Support and the table mounting clamps (left/right) from the table - if applicable. **STEP 2: Cleaning** **Available method: Manual cleaning - wipe system** **Cleaning equipment:** A. Disposable protective gloves for the cleaning operative. B. Damp, soft, non-abrasive non-linting cloth. **Note**: The same cloth should not be used from patient to patient. Replace cloth after each patient and dispose in a way that prevents users from cross infections. **Cleaning chemicals:** A. Use only isopropanol 70% **Cleaning process:** A. Check the conditions of use and safety warnings specified in the cleaning chemicals documentation. Apply the rules for the safe use of cleaning products. Ensure appropriate environmental conditions during cleaning. B. Apply the agent by spraying or moistened cloth. Use the amount of cleaning agent and the required contact time according to the conditions of use specified by the agent manufacturer.

C. Wipe the device and lead wires with a damp, soft, non-abrasive non-linting cloth.
D. Clean thoroughly all elements and surfaces that are dirty and may have direct contact with the patient and user.

Note: Clean the display screen with a clean cloth with an agent containing a solution of 70% isopropanol.

Note: Particular attention is required in hard-to-reach gaps and cavities where contaminants may accumulate.

Warning: Never use cleaning detergents that contain active oxygen or chlorine, as they may cause surface damage.

Prohibited method: Manual cleaning - immersive
Any immersive methods of cleaning are not allowed.
Prohibited method: Automated cleaning
Automated methods of cleaning are not allowed.

STEP 3: Disinfection

Disinfection equipment:

A. Disinfection may be carried out concurrently with the cleaning process. Apply the process equipment indicated in the cleaning section.

Disinfection chemicals:

A. Disinfection may be carried out concurrently with the cleaning process. Apply the chemicals indicated in the cleaning section.

Disinfection process:

A. Disinfection may be carried out concurrently with the cleaning process.

Prohibited method: Manual disinfection - immersion systems
Immersion systems of disinfection are not allowed.

Prohibited method: Automated chemical, thermal or other automated disinfection
Automated methods of disinfection are not allowed.

STEP 4: Drying

Drying equipment:

A. Natural drying or clean low-linting wipes.

Drying process:

A. Manual wiping and natural drying methods are recommended. Use only clean and low-linting wipes.

Note: Other drying methods may only be used when permissible environmental conditions remain met.

Warning: Do not exceed the maximum temperature that a medical device can withstand.

	Warning: Do not turn on the device until it dries completely. **STEP 5: Inspection and maintenance** A. Make sure there is no visible mechanical or other damages. Residues of cleaning agents and cleaning cloths on the device are unacceptable. B. Connect the main power to the device (by plugging the AC cable - professional use or using fuse switch disconnector in home healthcare environment), turn ON and check if the device starts correctly. **Note**: Inspections and maintenance of the device are performed in accordance with manufacturer's guidelines. **STEP 6: Packaging** Before packing the device, all accessories should be cleaned, disinfected and dried. **Note**: Details of packaging are described in chapter **18.7 Storage and transportation instructions**. **STEP 7: Storage** Use manufacturers defined permissible range of humidity and temperature conditions. When not in use for a long time, protect the device from contamination and other external factors. Store the device in its original packaging in a place that ensures safe and clean storage. **Note**: Details of storage are described in chapter **18.7 Storage and transportation instructions**. **STEP 8: Transportation** **Transport to point of use** Before transportation devices and extensions should be cleaned and disinfected. **Shipping outside facility** Before transportation the device should be cleaned and disinfected also for service and maintenance purposes. It is advisable to use the original, undamaged packaging to ensure transport safety and protect the device and the accessories from contamination. Note: Details of storage and transportation are described in chapter **18.7 Storage and transportation instructions**.
Reusable EMS electrodes	Follow the electrode manufacturer's instructions on the packaging/label or in the accompanying documentation.



Never clean Meissa OT with mains power ON! This may result in electric shock or short circuit the electronics inside.

Never use running water or other fluids for cleaning.

Do not sterilize. The device is neither intended to be sterilized nor supplied sterile.

Never use cleaning detergents that contain active oxygen or chlorine, as they may cause surface damage.

For the best cleaning experience, the manufacturer advises using a high-level disinfectant that can handle both bacterial and viral contaminations. An example is Amity International's Virusolve+ products, available in both spray form (excellent for extension grips) and wipes (ideal for chassis and metal parts).

When using high-level disinfectants, always follow the safety guidelines. Always read and adhere to the information provided with the substance.

Meissa OT is used for multiple patients, Therefore, please follow these guidelines:

1. Clean Meissa OT, the cables, and accessories after every use and before first use each day, according to the instructions above.
2. Consider using multiple extensions to limit exposure between patients.
3. Ensure that Meissa OT and its accessories are dried before storage or reuse.
4. Store according to the instructions provided in chapter **18.7 Storage and transportation instructions**.

No substances emitted by the device were detected in any material during its operational life, including the disinfection and cleaning processes.

Use only cleaning and disinfecting agents recommended by device manufacturer.

Cleaning and disinfection are required after each therapy and after each patient. Cleaning is required after each therapy even when the device is used only by one patient.

The device should be cleaned and disinfected before submission for service or repair to prevent cross-contamination and health risks to service personnel.

Please remember the annual maintenance of the device as further specified in section **7.11 Annual maintenance**.

20. Data protection

20.1 End user license agreement (EULA)

To provide services using Meissa OT device, the user will be required to sign an End User License Agreement (EULA) with **EGZO**Tech to regulate legal obligations between **EGZO**Tech and the user. The EULA can be found here https://support.egzotech.com/terms-and-conditions.

20.2 Data retention

EGZOTech reserves the right to retain collected data for a minimum period of 10 years from the cessation of manufacturing of the last Meissa OT device, in accordance with the requirements of Regulation (EU) 2017/745.

21. Declaration of Conformity and compliance statements

21.1 Declaration of Conformity

We hereby declare that Meissa OT complies with Regulation (EU) 2017/745 of the European Parliament and of the Council of April 5, 2017, on medical devices.

Classification: Class IIa, rule 9, according to Annex VIII of MDR Regulation.

This product meets all relevant European and international standards. All applicable requirements are listed in the Declaration of Conformity of the device.

Meissa OT is intended for use in the electromagnetic environment specified below. The customer or the user of Meissa OT should ensure it is used in such an environment.

Meissa OT complies with the electromagnetic compatibility requirements for emissions and immunity specified in the tables below. Users must adhere to the electromagnetic environment guidance and any deviations from the collateral standards specified. For necessary instructions on maintaining basic safety and essential performance in relation to electromagnetic disturbances and expected service life, please refer to the general warnings described in this manual.

21.2 Manufacturer's declaration – electromagnetic emissions

Guidance and manufacturer's declaration - electromagnetic emissions		
Emissions test	**Compliance**	**Electromagnetic environment - guidance**
RF emissions CISPR 11	Group 1	Meissa OT uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	Meissa OT is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Complies	

21.3 Manufacturer's declaration – electromagnetic immunity

Guidance and manufacturer's declaration - electromagnetic immunity		
Immunity test	**IEC 60601-1-2 test level - the device is tested to compliance level**	**Electromagnetic environment - guidance**
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 15 kV air	The floor should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply line; repetition freq. 100 kHz	Mains power quality should be that of a home, typical commercial or hospital environment.

<table>
<tr><td>Surge
IEC 61000-4-5</td><td>± 1 kV differential mode
± 2 kV common mode</td><td>Mains power quality should be that of a home, typical commercial or hospital environment.</td></tr>
<tr><td>Voltage dips, short interruptions and voltage variations on power supply input lines
IEC 61000-4-11</td><td>0% U_T; 0.5 cycle
at 0°, 45°, 90°, 135°, 180°, 225°, 270° & 315°

0% U_T; 1 cycle and
70% U_T; 25/30 cycles
single phase: at 0°
0% U_T; 250/300 cycle</td><td>Mains power quality should be that of a home, typical commercial or hospital environment.
If the user of the device requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power source.</td></tr>
<tr><td>Power frequency (50/60 Hz) magnetic field
IEC 61000-4-8</td><td>30 A/m</td><td>Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.</td></tr>
<tr><td>Conducted RF
IEC 61000-4-6</td><td>3 Vrms
150 kHz to 80 MHz

6 Vrms
in ISM bands between
150 kHz and 80 MHz</td><td rowspan="2">Portable and mobile RF communications equipment should be used no closer to any part of the device including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.
Recommended separation distance $d = \left[\frac{3.5}{V_1}\right]\sqrt{P}$
For 80 MHz to 800 MHz: $d = \left[\frac{3.5}{E_1}\right]\sqrt{P}$
For 800 MHz to 2,5 GHz: $d = \left[\frac{7}{E_1}\right]\sqrt{P}$
Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d in the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, [a] should be less than the compliance level in each frequency range. [b] Interference may occur in the vicinity of equipment marked with the following symbol:</td></tr>
<tr><td>Radiated RF
IEC 61000-4-3</td><td>3 V/m
80 MHz to 2.7 GHz
(Professional Healthcare)

10 V/m
80 MHz to 2.7 GHz
(Home Healthcare)</td></tr>
<tr><td colspan="3">NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</td></tr>
<tr><td colspan="3">[a] Field strengths from fixed transmitters, such as base stations for radio (mobile/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered, if the measured field strength in the location in which the [ME EQUIPMENT/SYSTEM] is used exceeds the applicable RF compliance level above, the [ME EQUIPMENT/SYSTEM] should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the [ME EQUIPMENT/SYSTEM].
[b] Over the frequency range 150 kHz to 80 MHz, field strengths should be less than [V1] V/m.</td></tr>
</table>

Guidance and manufacturer's declaration - immunity to RF wireless communications equipment					
Test f (MHz)	**Band (MHz)**	**Service**	**Modulation**	**Max Power (W)**	**Immunity test level (V/m)**
385	380 - 390	TETRA 400	Pulse modulation 18 Hz	1.8	27
450	430 - 470	GMRS 460, FRS 460	FM ± 5 kHz deviation 1 kHz sine wave	2	28
710	704 - 787	LTE Band 13, 17	Pulse modulation 217 Hz	0.2	9

745 780 810 870 930	800 - 960	GSM 800/900, TETRA 800, iDEN 820, CDMA 850, LTE Band 5	Pulse modulation 18 Hz	2	28
1 720 1 845 1 970	1700 - 1990	GSM 1800, CDMA 1900, GSM 1900, DECT, LTE Band 1, 3, 4, 25, IMTS	Pulse modulation 217 Hz	2	28
2 450	2400 - 2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation 217 Hz	2	28
5 240 5 500 5 785	5100 - 5800	WLAN 802.11 a/n	Pulse modulation 217 Hz	0.2	9
The Manufacturer is Compliant with all the above listed specifications.					
GUIDELINES: (a) For best performance of Meissa OT's wireless communication use Wi-Fi channels that are less populated by other Wi-Fi networks, (b) Other wireless communication may impact Meissa OT's essential performance, but not basic safety. (c) Please consider cybersecurity guidelines in this manual to prevent hacking.					
NOTE: (a) For some services, only the uplink frequencies are included. (b) The carrier shall be modulated using a 50% duty cycle square wave signal. (c) As an alternative to FM modulation, 50% pulse modulation at 18 Hz may be used because while it does not represent actual modulation, it would be the worst case.					

21.4 Recommended separation distances between portable and mobile RF communications equipment and Meissa OT

Meissa OT is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of Meissa OT can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and Meissa OT as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter (W)	**Separation distance according to frequency of transmitter (m)**		
	150 kHz to 80 MHz $d = \left[\frac{3,5}{V_1}\right]\sqrt{P}$	**80 MHz to 800 MHz** $d = \left[\frac{3,5}{E_1}\right]\sqrt{P}$	**800 MHz to 2,5 GHz** $d = \left[\frac{7}{E_1}\right]\sqrt{P}$
0.01	0.12	0.12	0.24
0.1	0.37	0.37	0.74
1	1.17	1.17	2.34
10	3.69	3.69	7.38
100	11.67	11.67	23.37

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

21.5 RF Radio Regulatory Statement

FCC Statement

This device complies with Part 15 of the FCC rules.

Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) This device must accept any interference received, including interference that may cause undesired operation.

Caution: Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device contains an RF modules:

- **FCC ID: 2AC7Z-ESP32WROVERE**
- **FCC ID: TFB-1004**

22. Meissa OT permanent installation protocol - home healthcare environment only

Service Location:

Address: _____

Date of Service: _____

Client details:

Name: _____

Address: _____

Phone Number: _____

Authorized service personnel (electrician) details:

Name: _____

Electrician qualification (e.g., SEP): _____

Phone Number: _____

Installation Confirmation

I, the undersigned electrician, confirm that the installation of the medical electrical equipment Meissa OT, serial number: _____, was completed in compliance with current regulations, safety standards and requirements specified in chapter **6.6 Use in home healthcare environment**. The client has been informed about the correct usage of the device.

Installation Details (according to IEC 60364)

Cable Type and Cross-Section: _____

Residual Current Device (RCD): Yes / No

Grounding Verification: Yes / No

Supply Voltage: _____

Type of Protection (Rated Current): _____

Does the installation meet manufacturer requirements and comply with relevant standards Yes / No

Control and Measuring Instrument Used for Verification

Manufacturer: _____

Model: _____

Serial Number: _____

Additional Notes

_____
_____
_____
_____
_____
_____
_____

Electrician's Signature: _____

Date: _____

Client's Signature: _____

Date: _____

Thank you for taking the time to read this manual!

Feel free to contact us at any time. We are here for you!

The service request form is available at:

HTTPS://SERVICE.EGZOTECH.COM

EGZOTech Sp. z o.o.
Romualda Traugutta 6H
44-100 Gliwice, POLAND
office@egzotech.com
+48 32 750 49 45