

Non-Enzymatic Glucose Sensor Based on Ni(OH)₂/NF Materials Using Different Pulse Voltammetry Technique

Do Trinh Xuan Minh¹, Dinh Hieu Trung^{1,2}, Tran Vu Diem Ngoc³, Chu Van Tuan⁴,
Nguyen Hai Ha⁴, Tran Tri Quang⁴, Chu Thi Xuan^{2,3*}, Dang Thi Thanh Le^{2,3},
Luc Nhu Quynh⁵, Nguyen Duc Hoa^{2,3}

¹School of Engineering Physics, Hanoi University of Science and Technology, Ha Noi, Vietnam

²International Training Institute for Materials Science (ITIMS),
Hanoi University of Science and Technology, Ha Noi, Vietnam

³School of Materials Science and Engineering, Hanoi University of Science and Technology, Ha Noi, Vietnam

⁴Hung Yen University of Technology and Education, Hung Yen, Vietnam

⁵Academy of Cryptography Techniques, Ha Noi, Vietnam

*Corresponding author email: xuan@itims.edu.vn

Abstract

Non-enzymatic glucose sensors have gained significant attention owing to their potential for accurate and cost-effective glucose detection. Nanomaterials play a pivotal role in enhancing performance of non-enzymatic glucose sensor. In this study, a novel non-enzymatic glucose sensor based on Ni(OH)₂/NF (nickel hydroxide/nickel foam) materials was developed using different pulse voltammetry technique. Chemical precipitation methods have been used to grow Ni(OH)₂ nanostructures directly on a nickel foam electrode. The characterization of the synthesized materials was performed through field emission scanning electron microscopy (FESEM), energy dispersive spectroscopy (EDX), and X-ray diffraction (XRD). The performance of the Ni(OH)₂/NF-based glucose sensor was evaluated through electrochemical measurements. Nanoscale hive-like structures of Ni(OH)₂ with a diameter ranging from 450 to 530 μm and a thickness of 20 nm were formed on the NF surface. The sensor exhibited good performance, displaying a high sensitivity of 8.42 mA·mM⁻¹·cm⁻² with a low detection limit of 0.84 μM. These results position the synthesized electrode as a promising contender for non-enzymatic electrochemical glucose sensors.

Keywords: Ni(OH)₂ nanostructures, Ni foam, non-enzymatic glucose sensing, electrochemical sensor, direct growth.

1. Introduction

Glucose serves as the primary molecular marker for diabetes monitoring and variations in its concentration hold paramount importance for human well-being. The precise quantification of glucose carries profound implications not only for proactive healthcare management but also extends its significance to future applications in preventive medicine, ensuring food safety, environmental surveillance, pharmaceutical analysis, and advancements in biotechnology [1]. Electrochemical analysis has gained recognition as a highly efficient and accurately calibrated technique for glucose detection. Currently, electrochemical glucose sensors can be categorized into two main types: non-enzyme sensors and enzyme sensors, based on the catalysts utilized in the detection process [2].

In recent years, electrochemical non-enzyme sensors have gained considerable prominence in the realm of glucose detection due to their cost-effectiveness, exceptional efficiency, resilience

against environmental fluctuation, and straightforward manufacturing processes [3]. A critical determinant for the performance of an exceptional electrochemical non-enzyme glucose sensor lies in the quality of its electro-catalysts, which should processes enduring stability, heightened sensitivity, and perfect selectivity. Non-enzymatic sensors exhibit noteworthy attributes such as heightened sensitivity, prolonged stability, rapid response times, and economical production [4]. Consequently, they have garnered escalating interest as compelling alternatives for surmounting the limitation inherent in enzymatic biosensors.

Many research groups have focused on the development of non-enzymatic sensors based on electrocatalytic oxidation of glucose on pure metal surfaces. Early investigations indicated that the oxidation of glucose on some noble metals, such as Pt and Au, behaved a sluggish kinetics and produced small faradaic currents [5]. In addition, noble metal surfaces proved susceptible to poisoning by adsorbed

intermediates and chloride ions, resulting in decreased sensitivity. Consequently, studying novel materials with suitable features has emerged as a pivotal factor in the construction of highly sensitive non-enzymatic glucose sensors.

In response to this challenge, numerous transition metal oxides or metal hydroxides, such as NiO, CuO, Co₃O₄ [6, 7], and Ni(OH)₂, [8, 9] have emerged as promising materials. Among these cost-effective candidates, nanostructures of Ni(OH)₂, a significant transition metal hydroxide, hold great promise as active electrode materials in non-enzymatic glucose electrochemical sensors [10]. Ni(OH)₂ materials can be fabricated via solgel synthesis [9], hydrothermal, and solvothermal methods [8] and then deposited on the electrode surface using a binder. Using a binder may increase electrode mass, modify electrode surface, or decrease charge transfer. To avoid using the binder, a simple method to grow Ni(OH)₂ directly on the electrode surface is in high demand. Direct growth of nanomaterials on the electrode surface offers several advantages, including enhanced materials-electrode bonding, fast charge transfer rate, and preservation of electrode surface.

In this paper, we reported a simple chemical precipitation method for the direct synthesis of nanostructured Ni(OH)₂ on nickel foam (NF). Nickel foam (NF) serves as an economical and versatile substrate characterized by its exceptional 3D porous architecture. This structure affords a substantial specific surface area, facilitating the deposition of nickel hydroxide and creating an abundance of sites crucial for the catalytic glucose reaction. Consequently, this configuration enhances the sensitivity of glucose detection, rendering nickel foam a promising substrate for glucose sensors. Furthermore, this method offers simplicity, cost-effectiveness, and the unique advantage of direct growth on electrode bases such as nickel foam. It is an environmentally friendly approach that can be easily implemented on a large scale, making it highly applicable across various fields.

2. Materials and Methods

2.1. Materials

All the chemical reagents employed in the experiment were of analytical grade, boasting a purity of 99.9%. Nickel(II) nitrate hexahydrate (Ni[NO₃]₂·6H₂O) and D(+)-glucose were produced from Merck KgaA (64271 Darmstadt, Germany). Hexamethylenetetramine (HMTA, C₆H₁₂N₄) was supplied by Tianjin Dengfeng Chemical Co., Ltd. Acetone (Xilong, China) and deionized water (DI) were also utilized in the experiments.

2.2. Synthesis of Ni(OH)₂ Nanostructure

The experimental procedure of Ni(OH)₂/NF electrode fabrication is shown in Fig. 1.




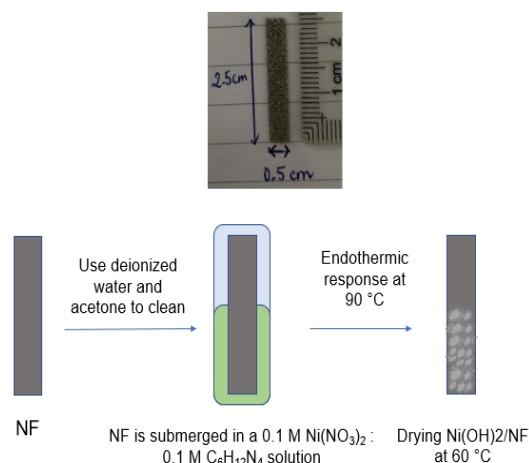


Fig. 1. Experiment procedure for fabrication of Ni(OH)₂/NF.

The substrate for the direct growth of Ni(OH)₂ nanostructures in this study was nickel foam (NF) with dimensions of 25 mm x 5 mm x 1.5 mm. The NF was cleaned in an ultrasonic bath containing acetone for 15 minutes, followed by another 15 minutes of immersion in deionized water. Subsequently, it was allowed to air dry for 30 minutes. In the next step, the cleaned NF was dipped in a solution composed 500ml of C₆H₁₂N₄ (HMTA) 0.5M and 500 ml of Ni(NO₃)₂ 0.5M. The synthesis of Ni(OH)₂ can be described through the following reactions:



The mixture was then heated in an oven at 90 °C for different times (10, 30, and 50 minutes). After the heating process, the fabricated structures were rinsed thoroughly using deionized water to remove any residual substances. Finally, the sensor was dried at 60 °C before being ready for measurement.

The morphological attributes and elemental composition of the constructed materials were assessed through the utilization of field-emission scanning electron microscopy (FE-SEM), energy dispersive spectroscopy (EDX), and X-ray diffraction (XRD).

2.3. Electrochemical Properties of Ni(OH)₂ and Glucose Measurement

All electrochemical measurements were performed in NaOH solution at ambient room temperature, employing three electrode system: Ag/AgCl as reference electrode, Pt wire as counter electrode, and Ni(OH)₂/NF as working electrode. Electrochemical properties of the fabricated Ni(OH)₂/NF electrode were characterized using cyclic voltammetry (CV) technique. The determination of

glucose concentrations was effectuated using differential pulse voltammetry (DPV).

3. Results and Discussion

3.1. Morphologies of the Ni(OH)₂/NF Materials

Fig. 2 delineates the FESEM images of the NF electrode and the synthesized Ni(OH)₂ nanostructures with various synthesized durations, corresponding to the samples of Ni(OH)₂ - 10m, Ni(OH)₂ - 30m, and Ni(OH)₂ - 50m. As shown in Fig 2a, no nanostructures were observed on the flat surface of the NF electrode. In contrast, following the formation of Ni(OH)₂, the substrate was covered with nanoscale hive-like structures (Fig. 2b-d). The samples manifest relatively uniform morphological features. The average diameter of pores on the electrode surface increases from 450 nm to 530 nm as synthesis time increases from 10 to 30min. This observed phenomenon is likely attributable to the progressive evolution of funnel-shaped pore structures over temporal progression. The thickness of the pore walls was estimated to be about 20 nm. The growth of nanohive structures of Ni(OH)₂ with very thin walls on NF electrode is favorable for the sensor, especially for an electrochemical sensor thanks to maximum adsorption ability. In addition, the direct growth of nanostructures on the electrode surface allows to avoid using extra binder, high temperature, or extra conductor.

3.2. Composition of the Ni(OH)₂/NF Materials

In order to analyse the composition of the synthesized materials, EDX technique was used. As shown in Fig. 3, Ni(OH)₂/NF samples primarily comprised of O (60.21%), C (28.36%), and Ni (11.42%). The presence of C can be attributed to Hexamethylenetetramine (HMTA, C₆H₁₂N₄) remaining in the sample, potential contamination from hydrocarbon compounds prevalent within the laboratory environment or arising from surface adsorption. Meanwhile, constituents' Ni and O are attributed to the Ni(OH)₂ sample. The prominent peaks of Ni, O, and C elements are clearly visible in the EDX spectrum, confirming the presence of Ni(OH)₂ structures atop the NF.

To ascertain the crystal structure of the electrode as it was manufactured, an XRD measurement was performed. The XRD patterns of Ni(OH)₂/NF are shown in Fig. 4. The characteristic peaks located at 45°, 52.7°, and 77° can be assigned to the (111), (200), (220) crystallographic planes of face-centered-cubic Ni crystal structure, respectively, (JCPDS 04-850).

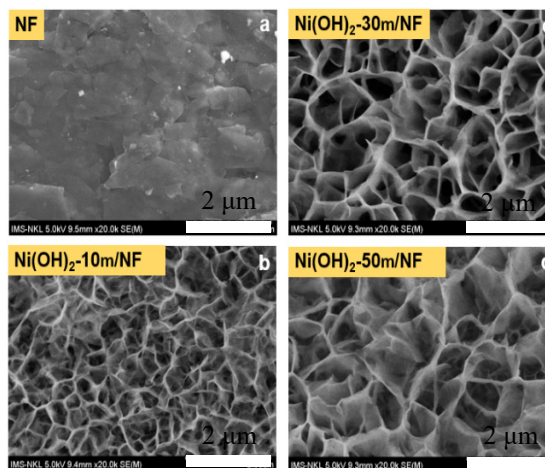


Fig. 2. FE-SEM images of (a) the bare NF and (b-d) the Ni(OH)₂/NF electrodes.

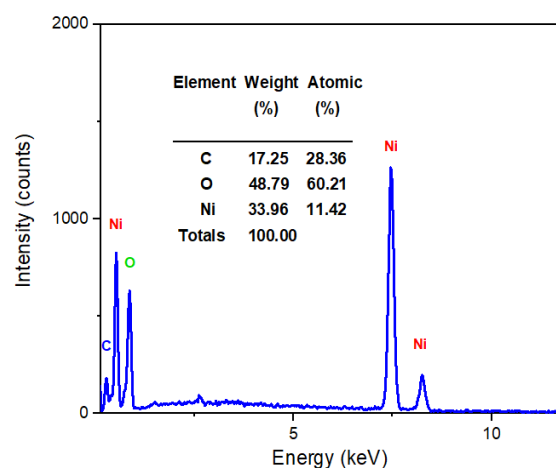


Fig. 3. EDX spectrum of Ni(OH)₂/NF.

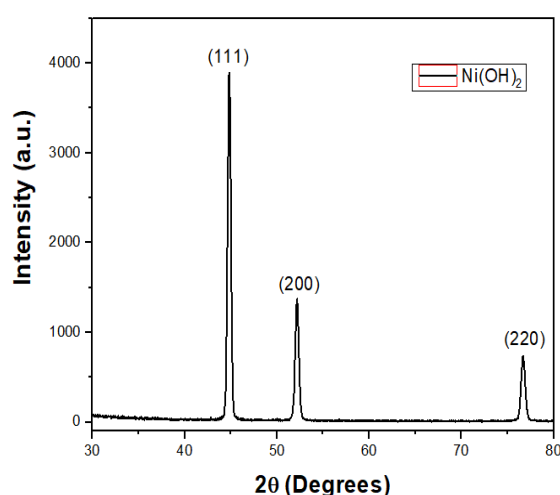


Fig. 4. X-ray diffraction patterns of Ni(OH)₂/NF films on Ni foam substrates.

3.3 Cyclic Voltammetry Measurement of the Synthesized Materials in Alkaline Medium

Fig. 5a, 5b, and 5c show the CV curves of the as-prepared Ni(OH)₂/NF-10m, Ni(OH)₂/NF-30m and Ni(OH)₂/NF-50m electrodes, respectively, in a potential range from -1.2 V to 1.6 V at a scan rate of 10 mV/s in a 0.1M NaOH solution. As shown in Fig. 5, anodic and cathodic peaks at potentials of 0.55 V and 0.2 V, respectively, representing the oxidation and reduction of the redox couple

Ni²⁺/Ni³⁺, were observed.

In order to assess the reproducibility of electrodes, four distinct Ni(OH)₂/NF electrodes that were fabricated under identical conditions were evaluated. The obtained results, as depicted in Fig. 5a, 5b, 5c, indicate that the variances observed in the cyclic voltammetry (CV) curves among the four sensors are minimal and insignificant. These results indicate that the fabricated Ni(OH)₂/NF electrodes are stable for glucose measurement.

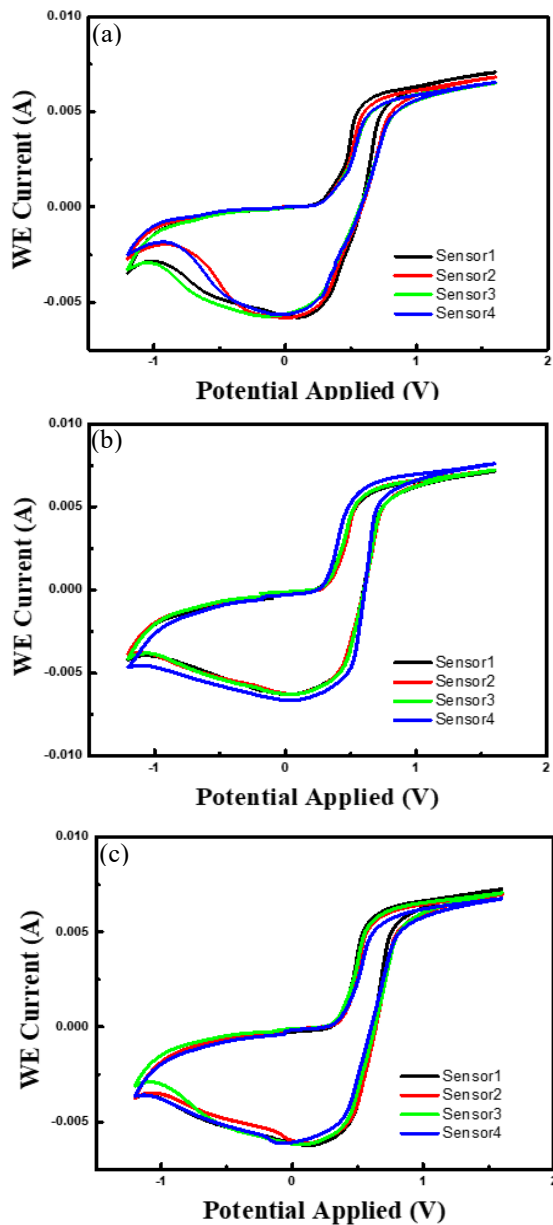


Fig. 5. CV curves of the a) Ni(OH)₂/NF-10m, b)Ni(OH)₂/NF-30m, c) Ni(OH)₂/NF-50m electrodes at a scan rate of 10 mV/s in 0.1 M NaOH.

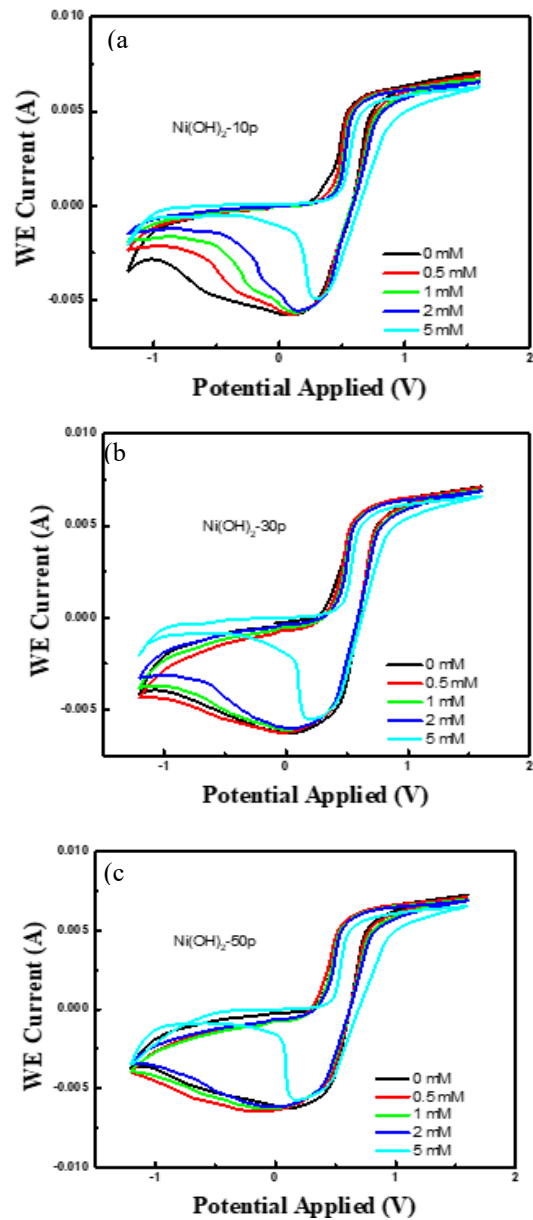


Fig. 6. CVs curves of (a) Ni(OH)₂/NF-10m, (b)Ni(OH)₂/NF-30m, (c) Ni(OH)₂/NF-50m electrodes in 20 mL NaOH 0.1M with glucose concentration from 0 to 5 mM.

3.4. Glucose Measurement

In order to test the sensitivity of the Ni(OH)₂/NF electrode to glucose, the cyclic voltammetry method was used. Fig. 6 presents the CV curves with different concentrations of glucose from 0 to 5 mM of three electrodes: Ni(OH)₂/NF-10m, Ni(OH)₂/NF-30m, and Ni(OH)₂/NF-50m in 0.1M NaOH solution at a scan rate of 10 mV/s.

The findings illustrated in Fig. 6a reveal that as the glucose concentration increases from 0 to 5 mM, there is a gradual reduction observed in both the cathodic and anodic peak currents. Notably, the response of the cathodic and anodic peaks remains relatively unchanged when glucose concentrations oscillate within the range of 0 to 2 mM for the Ni(OH)₂/NF-30m and Ni(OH)₂/NF-50m electrodes (Fig. 6b,c). It is only at the glucose concentration of 5 mM that discernible alterations in the cathodic and anodic peaks become apparent. Evidently, the Ni(OH)₂/NF-10m electrode demonstrates enhanced responsiveness to glucose, particularly at lower concentrations below 2 mM. The Ni(OH)₂/NF-10m electrode was chosen for further examination.

To further investigate the electrocatalytic activity of Ni(OH)₂/NF-10m for glucose oxidation, the DPV technique was used. DPV measurements were conducted to detect glucose with a concentration range from 0 to 5 mM in 0.1 M NaOH. Fig. 7a distinctly illustrates the progressive diminution in peak current as the glucose concentration escalates from 0 to 5 mM. The relationship between the response current and glucose concentration is expounded further within the calibration plot, as shown in Fig. 7b. The observed data

indicates a consistent reduction in current as the concentration of glucose increases. This relationship can be mathematically represented by the following equation, which describes a linear decrease:

$$I \text{ (mA)} = 0.00115 - 5.47224 * C_G \quad (1)$$

where C_G represents glucose concentration, measured in mM. The coefficient of determination, often denoted R^2 , is approximately 0.9918. The sensitivity, determined by dividing the slope by the working electrode area (0.65 cm²), is 8.42 mA.mM⁻¹.cm⁻². The detection limit, as established using a signal-to-noise ratio of three, is 0.84 μM [11]. The produced Ni(OH)₂/NF electrodes, exhibiting elevated sensitivity, rapid responsibility, and low limit of detection, are assessed as promising candidates for practical applications.

A comparison of our findings with recent publications concerning glucose sensors employing nickel foam substrates or Ni(OH)₂ materials is presented in Table 1. Among the published nickel-based non-enzymatic glucose sensors, the electrode featuring ultrathin walls, measuring approximately 20 nm, composed of Ni(OH)₂ nanohives atop a remarkably conductive nickel foam substrate stands out as a prime example of heightened sensitivity. This elevation in sensitivity is attributed to the augmented surface area conferred by the porosity intrinsic of Ni(OH)₂ nanohives. Notably, in relation to the linear range of glucose quantification, our finding is quite extensive, measuring from 0.05 to 5 mM. The results indicate that the Ni(OH)₂/NF electrode is capable of detecting glucose in an alkaline solution.

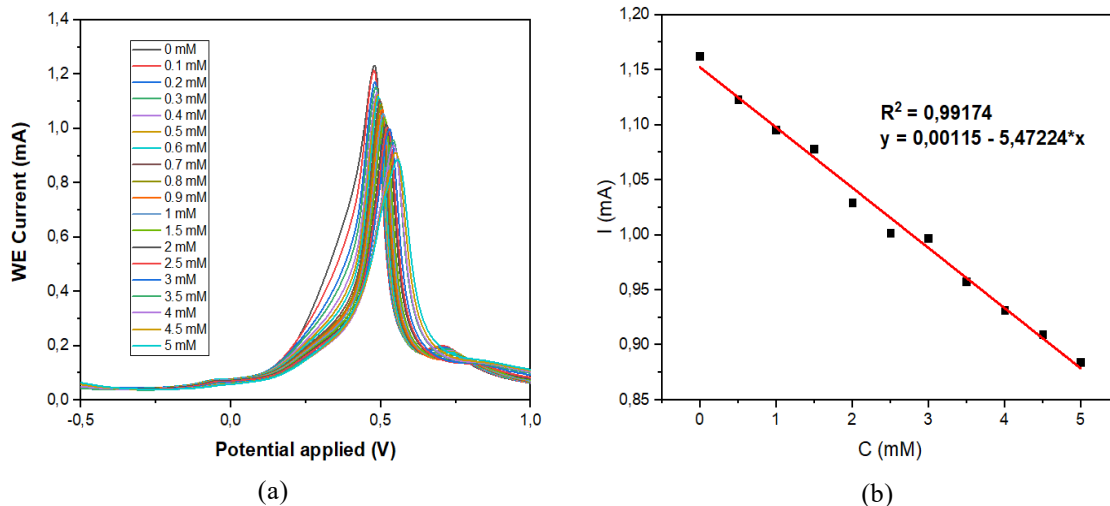


Fig. 7. a) DPV curve of Ni(OH)₂/NF-10m working electrode in 0.1 M NaOH containing glucose with the concentration range from 0 mM to 5 mM at a scan rate of 50 mV/s vs. Ag/AgCl and b) the calibration plot of response current vs. glucose concentration.

Table 1. Performance comparison of various glucose sensors

Materials	Sensitivity (mA mM ⁻¹ cm ⁻²)	Limit of detection (μM)	Linear range (mM)	Ref
NiCo ₂ O ₄ @Ppy/NF	3.06	0.22	0.001-20	[10]
Ni(OH) ₂ nanowires/NF	1.60	1	0.1-6	[12]
Ni(OH) ₂ nanosheet/Ni	1.13	1	0.002-0.04	[13]
Ni(OH) ₂ NPs/NF	1.95	0.16	0-6	[14]
Ni(OH) ₂ /PGE	0.948	2	0.004-3.5	[15]
Ni(OH) ₂ /TiO ₂	0.192	8	0.03-14	[16]
Ni(OH) ₂ /NF	8.42	0.84	0.05-5	This work

6. Conclusion

A simple and cost-effective chemical process was employed to successfully synthesize Ni(OH)₂ porous nanostructures directly on the surface of a nickel foam substrate. These fabricated electrodes were then utilized to measure glucose concentration in an alkaline medium at room temperature using CV and DPV methods. The non-enzymatic glucose sensors based on the Ni(OH)₂-coated nickel foam demonstrated excellent performance characteristics. They exhibited remarkable repeatability, high sensitivity (8.42 mA.mM⁻¹.cm⁻²), and a low limit of detection (0.84 μM). These outcomes underscore the substantial promise of the synthesized Ni(OH)₂-coated nickel foam electrodes for application in non-enzymatic glucose electrochemical sensors, particularly in clinical medical settings.

Acknowledgments

This research is funded by the Ministry of Education and Training (MOET) under project number B2022-BKA-25 CTVL.

Declaration of Competing Interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

References

- [1] M. Chawla, B. Pramanick, J. K. Randhawa, and P. F. Siril, Effect of composition and calcination on the enzymeless glucose detection of Cu-Ag bimetallic nanocomposites, *Mater Today Commun*, vol. 26, p. 101815, 2021.
<https://doi.org/10.1016/j.mtcomm.2020.101815>
- [2] G. A. Naikoo *et al.*, Fourth-generation glucose sensors composed of copper nanostructures for diabetes management: A critical review, *Bioengineering and Translational Medicine*, vol. 7, no. 1. John Wiley and Sons Inc, Jan. 01, 2022.

- [3] K. E. Toghiani and R. G. Compton, Electrochemical non-enzymatic glucose sensors: A perspective and an evaluation, *Int J Electrochem Sci*, vol. 5, no. 9, pp. 1246-1301, 2010.
[https://doi.org/10.1016/S1452-3981\(23\)15359-4](https://doi.org/10.1016/S1452-3981(23)15359-4)
- [4] M. Chawla, B. Pramanick, J. K. Randhawa, and P. F. Siril, Effect of composition and calcination on the enzymeless glucose detection of Cu-Ag bimetallic nanocomposites, *Mater Today Commun*, vol. 26, p. 101815, 2021.
<https://doi.org/10.1016/j.mtcomm.2020.101815>
- [5] L. Chen *et al.*, Preparation of Ni(OH)₂ nanoplatelet/electrospun carbon nanofiber hybrids for highly sensitive nonenzymatic glucose sensors, *RSC Adv*, vol. 7, no. 31, pp. 19345-19352, 2017.
<https://doi.org/10.1039/C7RA02064C>
- [6] C. Zhao, X. Wu, P. Li, C. Zhao, and X. Qian, Hydrothermal deposition of CuO/rGO/Cu₂O nanocomposite on copper foil for sensitive nonenzymatic voltammetric determination of glucose and hydrogen peroxide, *Microchimica Acta*, vol. 184, no. 7, pp. 2341-2348, 2017.
<https://doi.org/10.1007/s00604-017-2229-9>
- [7] J. Qian *et al.*, Non-enzymatic glucose sensor based on ZnO-CeO₂ whiskers, *Mater Chem Phys*, vol. 239, no. May 2019, p. 122051, 2020.
<https://doi.org/10.1016/j.matchemphys.2019.122051>
- [8] S. F. Alshareef, N. A. Alhebshi, K. Almashhori, H. S. Alshaikeid, and F. Al-hazmi, A ten-minute synthesis of α-Ni(OH)₂ nanoflakes assisted by microwave on flexible stainless-steel for energy storage devices, *Nanomaterials*, vol. 12, no. 11, Jun. 2022.
<https://doi.org/10.3390/nano12111911>
- [9] H. Yu *et al.*, A facile method for synthesis of Ni(OH)₂@xRF with excellent electrochemical performances, *Mater Lett*, vol. 273, p. 127867, Aug. 2020.
<https://doi.org/10.1016/j.matlet.2020.127867>
- [10] N. Pal, S. Banerjee, and A. Bhaumik, A facile route for the syntheses of Ni(OH)₂ and NiO nanostructures as

- potential candidates for non-enzymatic glucose sensor, *J Colloid Interface Sci*, vol. 516, pp. 121-127, 2018.
<https://doi.org/10.1016/j.jcis.2018.01.027>
- [11] N. Pal, S. Banerjee, and A. Bhaumik, A facile route for the syntheses of Ni(OH)₂ and NiO nanostructures as potential candidates for non-enzymatic glucose sensor, *J Colloid Interface Sci*, vol. 516, pp. 121-127, Apr. 2018.
<https://doi.org/10.1016/j.jcis.2018.01.027>
- [12] Q. Xiao, X. Wang, and S. Huang, Facile synthesis of Ni(OH)₂ nanowires on nickel foam via one step low-temperature hydrothermal route for non-enzymatic glucose sensor, *Mater Lett*, vol. 198, pp. 19-22, 2017.
<https://doi.org/10.1016/j.matlet.2017.03.172>
- [13] Y. Zhao *et al.*, Preparation of Ni(OH)₂ nanosheets on Ni foam via a direct precipitation method for a highly sensitive non-enzymatic glucose sensor, *RSC Adv*, vol. 5, no. 66, pp. 53665-53670, 2015.
<https://doi.org/10.1039/C5RA06664F>
- [14] C. W. Kung, Y. H. Cheng, and K. C. Ho, Single layer of nickel hydroxide nanoparticles covered on a porous Ni foam and its application for highly sensitive non-enzymatic glucose sensor, *Sens Actuators B Chem*, vol. 204, pp. 159-166, 2014.
<https://doi.org/10.1016/j.snb.2014.07.102>
- [15] M. L. Chelaghmia, M. Nacef, A. M. Affoune, M. Pontié, and T. Derabla, Facile Synthesis of Ni(OH)₂ Modified Disposable Pencil Graphite Electrode and its Application for Highly Sensitive Non-enzymatic Glucose Sensor, *Electroanalysis*, vol. 30, no. 6, pp. 1117-1124, 2018.
<https://doi.org/10.1002/elan.201800002>
- [16] A. Gao *et al.*, In situ synthesis of Ni(OH)₂/TiO₂ composite film on NiTi alloy for non-enzymatic glucose sensing, *Sens Actuators B Chem*, vol. 232, pp. 150-157, 2016.
<https://doi.org/10.1016/j.snb.2016.03.122>