

Comprehensive Analysis + Unknown Component Analysis of Vinyl Acetate Resins Using Pyrolysis GC-MS

Characteristic Component Extraction by Multiple Classification PCA and Component Identification by High Resolution MS -

Product used : Mass Spectrometer (MS)

[General]

Advances in mass spectrometry are enabling analysis of micro samples and unknown components that were not observable before. As the volume of information acquired from mass spectrometry increases, researchers are calling for simple techniques to analyze numerous components observed, and as a result, there is a rise in demand for comprehensive analytical techniques including multiple classification analysis.

In this work, we will introduce a new technique for non-target analysis, which combines comprehensive analysis using high resolution GC-TOFMS and unknown component analysis using soft ionization.

[Method]

As model samples, 6 commercial vinyl acetate resins (adhesives) were used. A gas chromatography time-of-flight mass spectrometer (GC-TOFMS) was used for measurement. Since emulsion samples including adhesives are difficult to analyze without preliminary treatment, the samples were subjected to pyrolysis.

The resulting data was analyzed by AnalyzePro (SpectralWorks) to compare multiple samples by PCA.

[Results]

A total of 6 vinyl acetate resin samples were analyzed by pyrolysis GC-EI TOFMS (n=3), and the resulting data was subjected to PCA by AnalyzerPro. The PCA score plot (Figure 1) shows that sample E was clearly separated at the 1st principal component axis and sample B at the 2nd principal component axis, respectively. Components contributing to each principal component were easily detected in the loading plot.

Among the components contributing to the separation at the secondary principal component axis (positive side), that is, characteristic components of sample B, the component at R.T. 4.55 min was analyzed in detail (data on the right side of Figure 2).

The NIST library search estimated that the component at R.T. 4.55 min was likely to be 2,2,4-Trimethyl-1,3-pentanediol diisobutyrate (molecular weight 286) with a match factor of 813. However, the FI mass spectrum of this component detected a base peak at m/z 217, and as a result, the molecular weight estimated in NIST library search differed significantly from the molecular weight estimated from the results of FI ionization. While the chemical structure of 2,2,4-Trimethyl-1,3-pentanediol diisobutyrate contains an ester group, FI ionization detected no ion that has an m/z equal to that. Ester group containing compounds are generally known to produce protonated molecules by FI ionization. Thus, it is likely that the component at R.T. 4.55 min is not the component estimated in NIST library search but is another component having a similar EI spectrum. Figure 3 shows the mass spectra of the component at R.T. 4.55 min acquired by EI and FI. Figure 4 shows the structural formula of 2,2,4-Trimethyl-1,3-pentanediol diisobutyrate. After examining the EI and FI data in detail, it was estimated that the component at R.T. 4.55 min has the structure shown in Figure 5. None of the major libraries provided by NIST included a component equal to this structure.

PCA is an effective and efficient technique for the comprehensive analysis of GC-TOFMS data. Specifically, for multiple sample comparisons, use of score and loading plots makes it possible to examine the similarities between the samples and the characteristic components of each sample. Also, while the NIST library search is a powerful tool for identifying characteristic components of samples, combining NIST library searches with molecular weight information acquired by soft ionization such as FI makes it possible to identify components with a higher level of accuracy, preventing false identifications.

Table 1. Measurement Conditions

[Py-GC-TOFMS Conditions]

System	JMS-T200GC (JEOL)
Pyrolysis temp.	600°C
Ionization mode	EI+: 70 eV, 300 μ A FI+: -10 kV, 6 mA (Carbotec 5 μ m)
GC column	DB-5msUI (Agilent), 15 m x 0.25 mm, 0.25 μ m
Oven temp.	50°C (1 min) \rightarrow 30°C/min \rightarrow 330°C (1.7 min)
Inlet temperature	300°C
Inlet mode	Split 100:1
He flow	1.0 mL/min (Constant Flow)
m/z range	m/z 35-650
Spectrum recording speed	0.1 sec
Software	AnalyzerPro (SpectralWork)

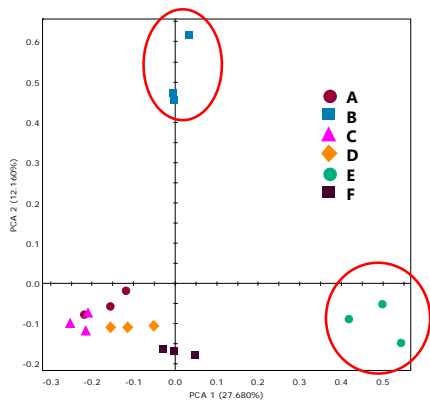


Figure 1. PCA score plot of polyvinyl acetate samples



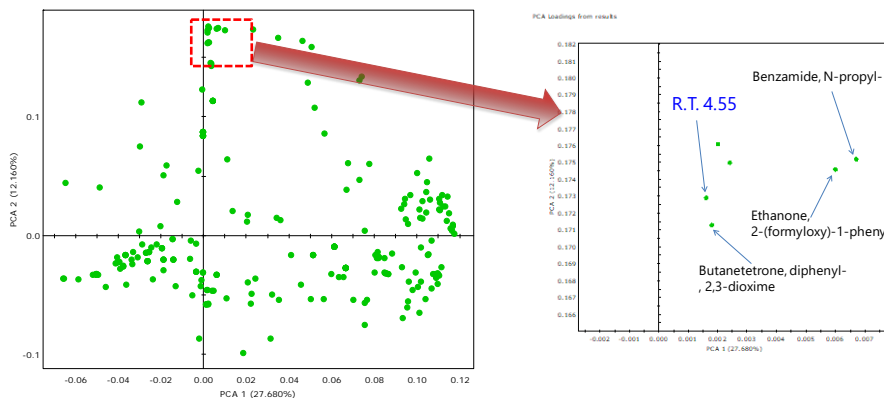


Figure 2. PCA loading plot of polyvinyl acetate samples

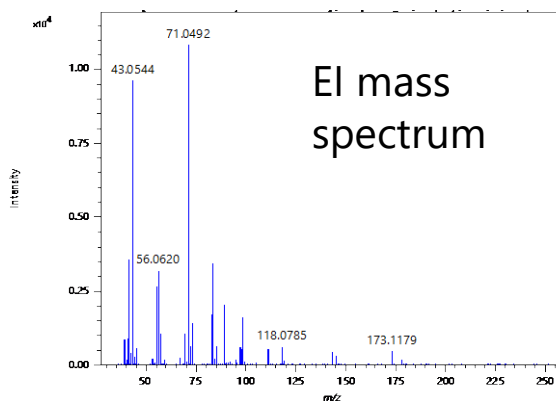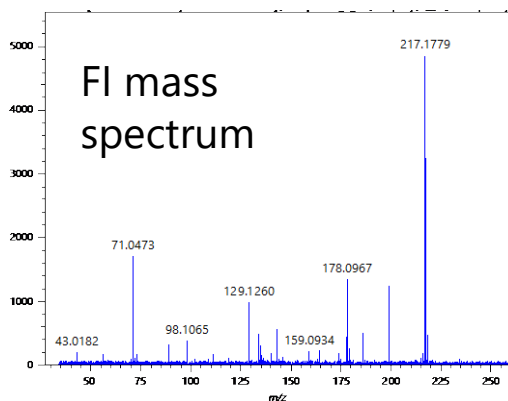

Mass	Formula	Calculated Mass	Mass Error [mDa]	DBE
217.178	C ₁₂ H ₂₅ O ₃	217.1798	-1.8	0.5

Mass	Formula	Calculated Mass	Mass Error [mDa]	DBE
43.0544	C ₃ H ₇	43.0542	0.2	0.5
56.0622	C ₄ H ₈	56.0621	0.1	1.0
71.0493	C ₄ H ₇ O	71.0491	0.2	1.5
83.0858	C ₆ H ₁₁	83.0855	0.3	1.5
89.0596	C ₄ H ₉ O ₂	89.0597	-0.1	0.5
98.1091	C ₇ H ₁₄	98.1090	0.1	1.0
111.1177	C ₈ H ₁₅	111.1168	0.9	1.5
143.1096	C ₈ H ₁₅ O ₂	143.1067	2.9	1.5
145.1246	C ₈ H ₁₇ O ₂	145.1223	2.3	0.5
173.1189	C ₉ H ₁₇ O ₃	173.1172	1.7	1.5

Figure 3. EI and FI mass spectra and exact mass analysis results for the unknown component (R.T. 4.55 min) in sample B

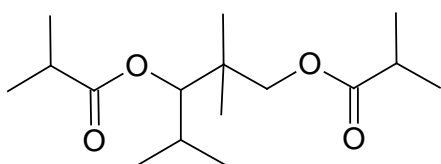


Figure 4. Structural formula of 2,2,4-Trimethyl-1,3-pentenediol diisobutyrate

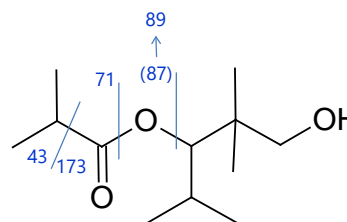


Figure 5. Estimated structural formula for the unknown component (R.T. 4.55 min) in sample B

Copyright © 2018 JEOL Ltd.

Certain products in this brochure are controlled under the "Foreign Exchange and Foreign Trade Law" of Japan in compliance with international security export control. JEOL Ltd. must provide the Japanese Government with "End-user's Statement of Assurance" and "End-use Certificate" in order to obtain the export license needed for export from Japan. If the product to be exported is in this category, the end user will be asked to fill in these certificate forms.



JEOL Ltd.

3-1-2 Musashino Akishima Tokyo 196-8558 Japan Sales Division Tel. +81-3-6262-3560 Fax. +81-3-6262-3577
www.jeol.com ISO 9001 • ISO 14001 Certified

• AUSTRALIA & NEW ZEALAND /JEOL(AUSTRALASIA) Pty.Ltd. Suite 1, L2 18 Aquatic Drive - Frenchs Forest NSW 2086 Australia • BELGIUM /JEOL (EUROPE) B.V. Planet II, Gebouw B Leuvensesteenweg 542, B-1830 Zaventem Belgium • BRAZIL /JEOL Brasil Instrumentos Cientificos Ltda. Av. Jabaquara, 2958 5º andar conjunto 52, 04046-500 Sao Paulo, SP Brazil • CANADA /JEOL CANADA, INC. 3275 1ere Rue, Local #8 St-Hubert, QC J3Y-8Y6, Canada • CHINA /JEOL(BEIJING) CO., LTD. Zhongkeziyuan Building South Tower 2F, Zhongguancun Nanshanjie Street No. 6, Haidian District, Beijing, P.R.China • EGYPT /JEOL SERVICE BUREAU 3rd Fl. Nile Center Bldg., Nawal Street, Dokki, (Cairo), Egypt • FRANCE /JEOL (EUROPE) SAS Espace Claude Monet, 1 Allée de Giverny 78290, Croissy-sur-Seine, France • GERMANY /JEOL (GERMANY) GmbH Gute Aenger 30 85356 Freising, Germany • GREAT BRITAIN & IRELAND /JEOL (U.K.) LTD. JEOL House, Silver Court, Watchmead, Welwyn Garden City, Herts AL7 1LT, U.K. • ITALY /JEOL (ITALIA) S.p.A. Palazzo Pacinotti - Milano 3 City, Via Ludovico il Moro, 6/A 20080 Basiglio(MI) Italy • KOREA /JEOL KOREA LTD. Dongwoo Bldg. 7F, 1443, Yangjae Daero, Gangdong-Gu, Seoul, 05355, Korea • MALAYSIA /JEOL(MALAYSIA) SDN.BHD. 508, Block A, Level 5, Kelana Business Center, 97, Jalan SS 7/2, Kelana Jaya, 47301 Petaling Jaya, Selangor, Malaysia • MEXICO /JEOL DE MEXICO S.A. DE C.V. Arkansas 11 Piso 2 Colonia Napoles Delegacion Benito Juarez, C.P. 03810 Mexico D.F., Mexico • RUSSIA /JEOL (RUS) LLC. Krasnoproletarskaya Street, 16, Bld. 2, 127473, Moscow, Russian Federation • SCANDINAVIA /SWEDEN JEOL (Nordic) AB Hammarbacken 6A, Box 716, 191 27 Sollentuna Sweden • SINGAPORE /JEOL ASIA PTE.LTD. 2 Corporation Road #01-12 Corporation Place Singapore 618494 • TAIWAN /JIE DONG CO., LTD. 7F, 112, Chung Hsiao East Road, Section 1, Taipei, Taiwan 10023 (R.O.C.) • THE NETHERLANDS /JEOL (EUROPE) B.V. Lireweg 4, NL-2153 PH Nieuw-Vennep, The Netherlands • USA /JEOL USA, INC. 11 Dearborn Road, Peabody, MA 01960, U.S.A.