



# Refrigerants

## Application Note

Environmental

### Authors

Agilent Technologies, Inc.

### Introduction

Fast GC analysis of halogenated refrigerant mixtures is achieved in less than 50 seconds using an Agilent PoraPLOT U column and Agilent 490 Micro GC.



**Agilent Technologies**


## Conditions

Technique : Micro GC  
Column : Agilent PoraPLOT U, 0.25 mm x 10 m fused silica  
Temperature : 119 °C  
Carrier Gas : Helium  
Pressure program : 100 kPa, 5 sec, → 250 kPa, 200 kPa/min  
Injector : chip injector heated, 100 °C  
Injection time : 5 ms  
Detector : chip TCD, Sensitivity: med  
Concentration Range : % level

Courtesy : Mario Voglino  
Stuart Wallman,  
A-GAS (UK) Ltd

## Peak identification

1. air
2. CFC 32
3. CFC 143A
4. CFC 125
5. CFC 134A
6. CFC 22

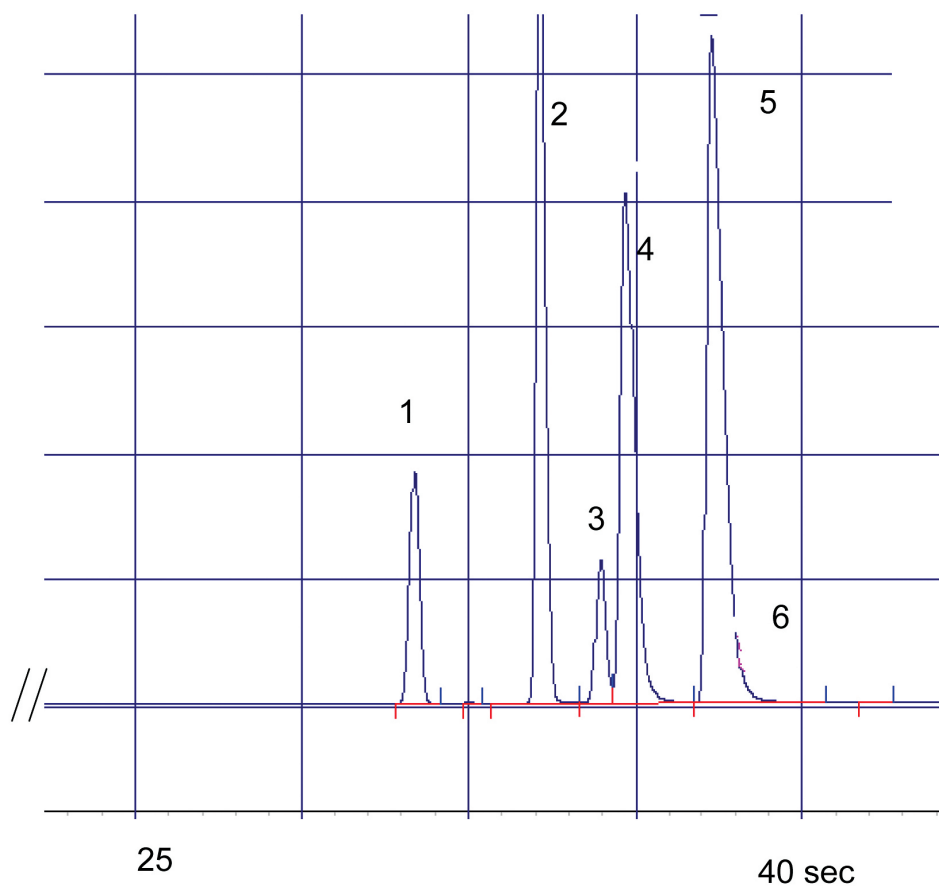

[www.agilent.com/chem](http://www.agilent.com/chem)

This information is subject to change without notice.

© Agilent Technologies, Inc. 2011

Printed in the USA

31 October, 2011

First published prior to 11 May, 2010

A01957



**Agilent Technologies**