

Differentiation of styrenic polymers using evolved gas analysis (EGA)-MS

[Background] Pyrolysis (Py)-GC/MS is commonly used to differentiate unknown polymeric materials. However, the pyrograms are often complex, which means that the data processing and polymer differentiation often requires an experienced analyst and time. There is an alternative to PY-GC/MS: evolved gas analysis (EGA)-MS. EGA-MS gives the analyst a thermal profile of the sample and the mass spectra of the components evolving from the sample as it is heated. 15 styrenic polymers, such as polystyrene (PS), copolymers of PS, and polymers of styrene derivatives, were analyzed using EGA-MS. The styrenic polymers were differentiated using the EGA thermogram and principal component analysis (PCA) of the EGA thermograms.

[Experimental] EGA-MS measurements were performed using a Multi-Shot Pyrolyzer (EGA/PY-3030D, Frontier Labs), which was directly interfaced to the split injector of a GC/MS system. A deactivated stainless steel capillary tube (L=2.5 m, id.=0.15 mm) was used to connect the GC injection port to the MS ion source. The average mass spectra of each styrenic polymer were stored in a mass spectral library (MS-Lib). In addition to the mass spectrum, profile parameters, such as peak apex temperature, higher and lower temperatures at half height, were used to assist in differentiating the various polymers.

[Results] First, the average mass spectrum of the unknown polymers were compared to the 15 spectra previously added to the MS-Lib library. If the match quality for a given unknown polymer was significantly higher than any of the other library entries, it was considered as 'identified'. However, some of the samples had very similar averaged mass spectra because the major pyrolyzate was styrene – see Fig. 1. For these unknowns, a PCA was performed using three parameters found in every EGA thermogram. In most cases, the choices could be narrowed down to a single candidate. For example, Fig. 1 shows that the EGA thermogram of the unknown sample is similar to those of No.5 (AS), No.6 (ABS) and No. 8 (AES). The match quality of the average mass spectrum for all three polymers is greater than 90%. Fig. 2 illustrates how PCA can be used to complement the library search results and facilitate the identification of the unknown polymer. This example illustrates how similar structures can be rapidly screened and differentiated using the averaged mass spectra of the thermograms obtained using EGA-MS and the PCA of the thermogram profile parameters. Using EGA-MS in lieu of, or as a complement to, PY-GC/MS improves laboratory productivity and the accuracy of the identification.

Averaged mass spectrum of main peak Thermogram

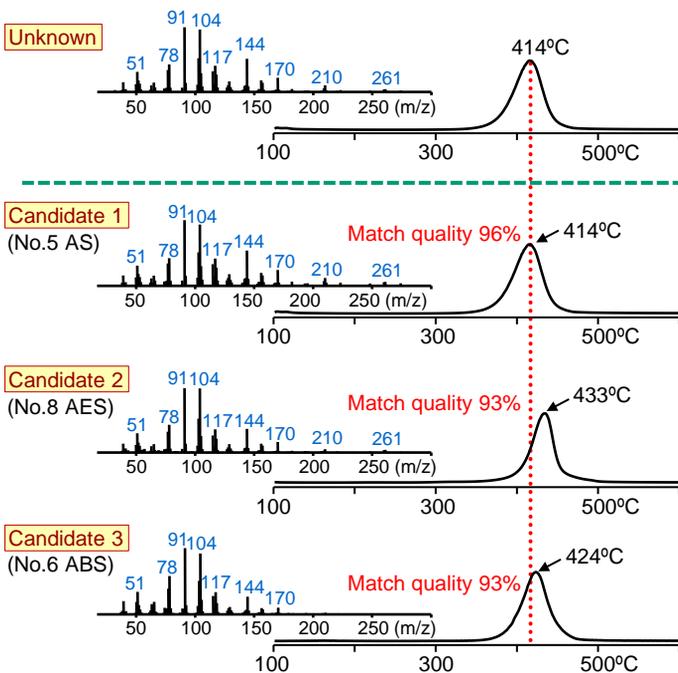


Fig. 1 Library search of an unknown using polystyrene MS Library

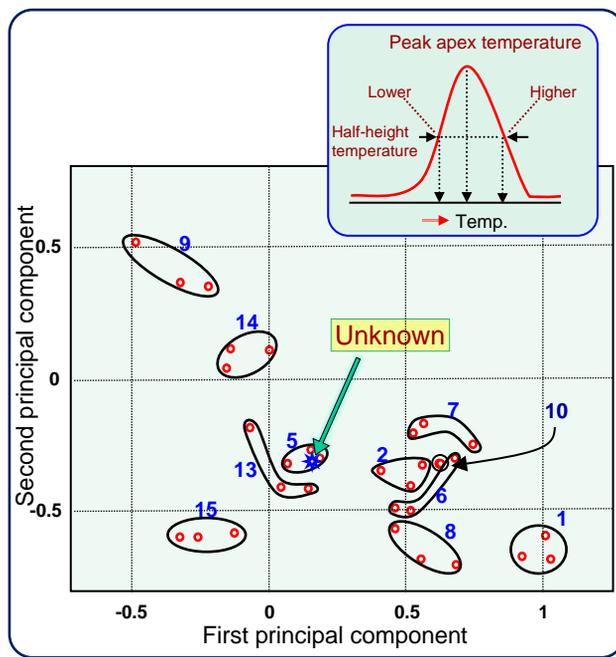


Fig. 2 Principal component analysis of thermogram shapes

Keyword : Forensic differentiation, F-Search, EGA-MS, PS, Averaged mass spectrum, Thermogram, PCA

Applications : General polymer analysis, Forensic investigation

Related technical notes : PYA1-067E, PYA3-012E, PYA3-013E, PYA3-017E

Please forward your inquiries via our web page or send us a fax message.

R&D and manufactured by :
Frontier Laboratories Ltd.

1-8-14 Saikon, Koriyama,
 Fukushima 963-8862 JAPAN
 Phone: (81)24-935-5100 Fax: (81)24-935-5102
<http://www.frontier-lab.com/>