


Fourier Transform Infrared Spectrophotometer

# IRSpirit-X Series



# IRSpirit™, **Ready to Run**

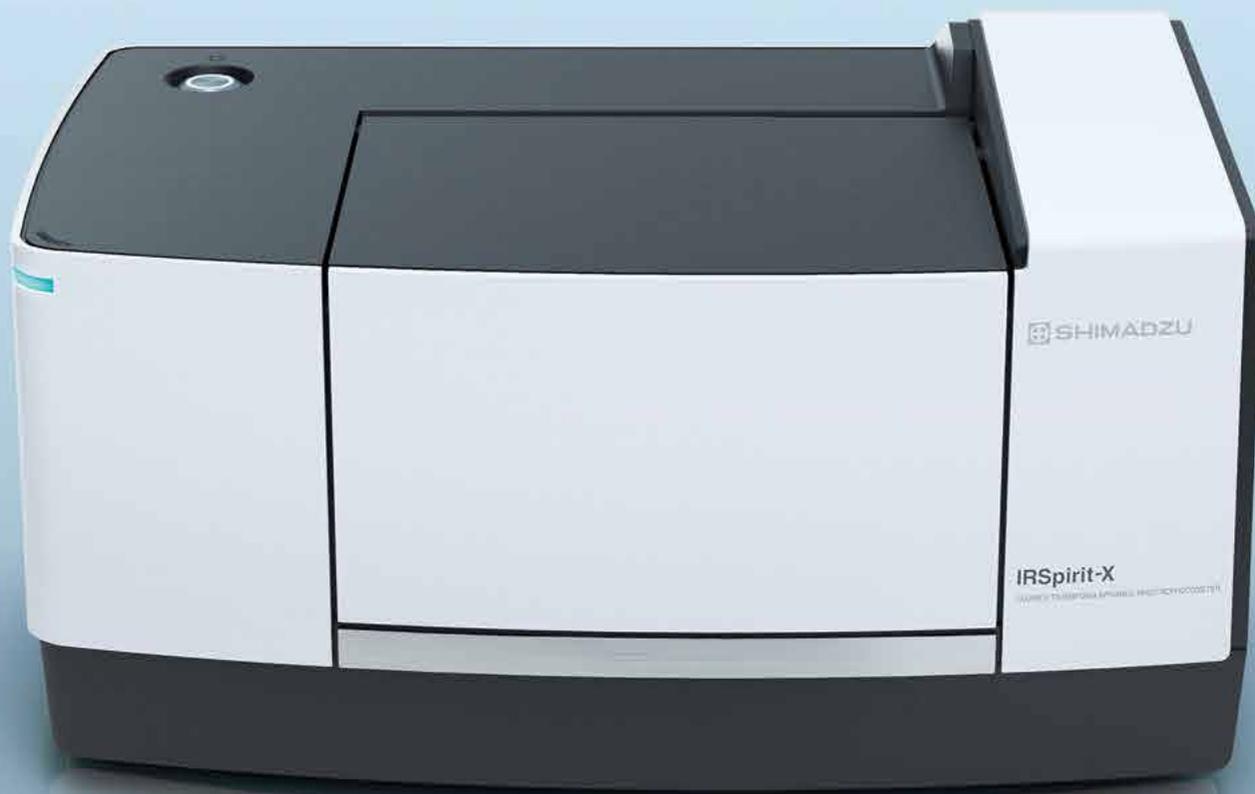

## **IRSpirit-X**

FOURIER TRANSFORM INFRARED SPECTROPHOTOMETER

## Space-Saving, Expandable

- Great for Small Lab Spaces
- Standard-Sized Sample Compartment in a Compact Bench

## FTIR Made Easier

- IR Pilot™ Pre-built Macro Program
- Spectrum Advisor Function
- Contaminant Analysis Program
- Identification Test Program

## Reliability to Deploy with Confidence

- Technology Inherited from Higher-End Models
  - Reliable Parts Come with a 10-Year Warranty
- Note: This warranty does not cover consumables, accessories other than the FTIR main unit, PCs and peripherals, instruction manuals, jigs, and labor charges for the second and subsequent years.
- High Durability Due to Humidity-Resistant Design
  - Internal Dehumidifier (Optional) Ensures Robustness
  - Instrument Status Monitoring

## Simple Operation, Confident Results

- Easy Macro – Just a Single Click Launches Routine Work
- Acquisition and Analysis of EDX and FTIR Data from a Single Computer

## Space-Saving, Expandable

### Great for Small Lab Spaces

There is a growing need for systems that can fit in tight spaces, like glove boxes and multiuse facilities, and the IRSpirit-X is perfect for those situation. Even in narrow spaces, samples can be measured with the unit positioned vertically (see images below). The start button is accessible and the humidity indicator is visible from both directions.

In addition, the ATR crystal and FTIR main unit are the same height. Therefore, samples can be placed directly on the ATR attachment, which is integrated with the sample compartment, which can eliminate the trouble of having to cut large samples.




Start Button

Humidity Indicator



## Standard-Sized Sample Compartment in a Compact Bench

In spite of a body size smaller than a piece of A3 paper, the sample compartment width is the same as on higher-end models. This makes it compatible with many Shimadzu and 3rd party accessories, allowing it to be used for a wide variety of applications.

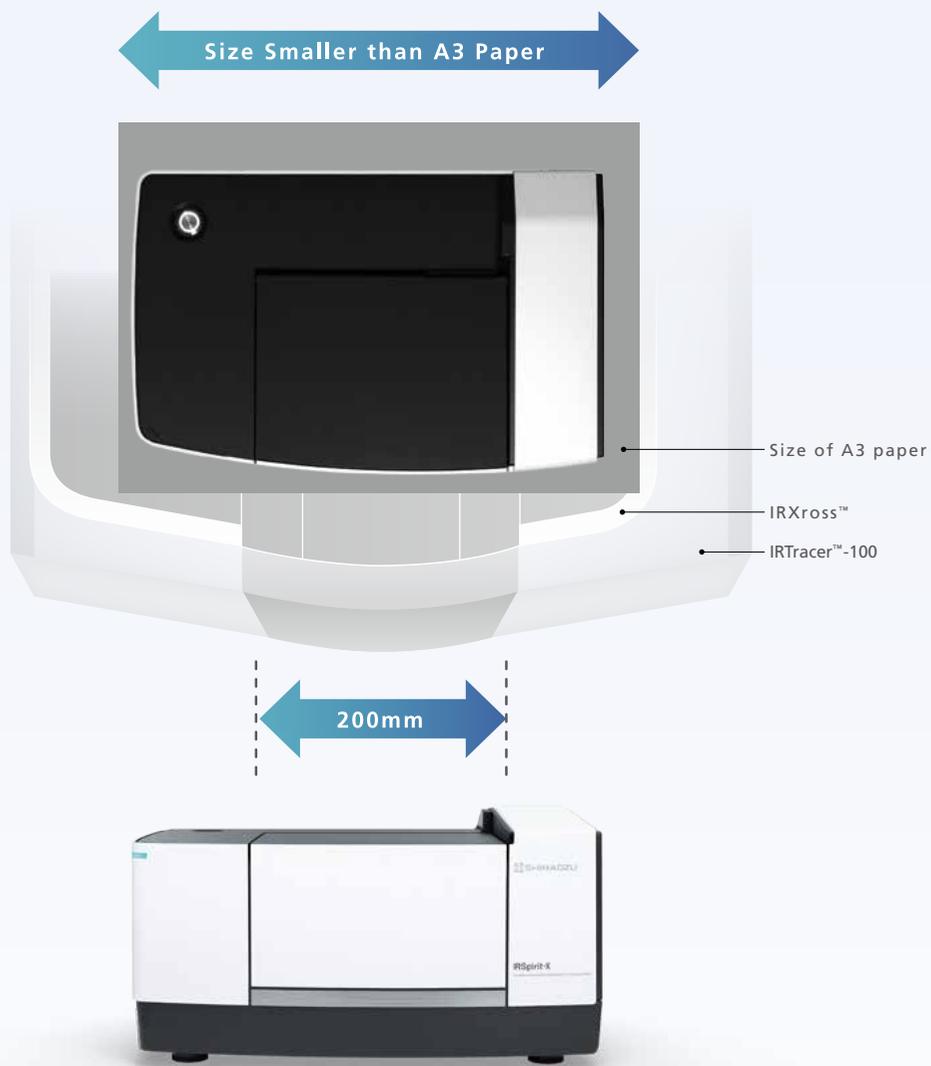

Fields	Applications	Contaminant analysis	Raw materials acceptance inspection	Identification tests	Quantitative analysis	Spectral analysis
Pharmaceuticals and life sciences		●	●	●	●	●
Chemicals and petroleum		●	●	●		●
Academia				●	●	●
Environmental		●			●	●

● : Applicable





## FTIR Made Easier

### IR Pilot™




IR Pilot offers a total of 23 application programs as standard, making it easy for operators with minimal FTIR experience to analyze samples by simply selecting the analysis purpose and accessory. There is no need to set parameters. Once a workflow has been determined, it can be recorded, which means that for analyses with the same procedures, the sequence from measurement to data analysis and printing can be performed with a few clicks.

\* Quantitative analysis function cannot be used when using IR Pilot with LabSolutions DB/CS.



## Spectrum Advisor Function (patent pending)

Corrective measures are proposed by comparing the measured spectrum to optimal spectrum examples. Troubleshooting advice is provided on scan parameters, accessories, and post-processing data. As a result, better quality data can be acquired.

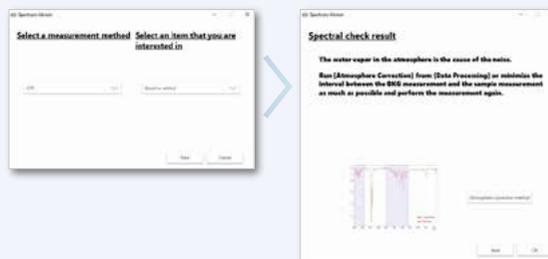

## Contaminant Analysis Program

The contaminant analysis program identifies measured contaminants using Shimadzu's proprietary identification algorithm (Japanese Patent No. 5205918) in combination with a spectral library containing more than 550 spectra for substances commonly detected as contaminants. After data analysis, it automatically makes a pass/fail judgment and creates a report. Even if the contaminant is a mixture, it searches for major and minor components and displays their ranks. Since the number of components in the mixture does not need to be specified, even operators with minimal infrared analysis experience can easily analyze samples. It takes just seconds between selecting the spectrum and displaying the analysis results.



## Identification Test Program

The identification test program calculates the difference in peak wavenumbers and peak ratio intensities between standard and test sample data, and then summarizes the pass/fail judgment results in a printed report. This program can be used if the standard is described in the national pharmacopoeia or official law. Spectra of 57 substances included in Japan's Specifications and Standards for Food Additives are also included in this program.




# Reliability to Deploy with Confidence

## Technology Inherited from Higher-End Models




Note:  
This warranty does not cover consumables, accessories other than the FTIR main unit, PCs and peripherals, instruction manuals, jigs, and labor charges for the second and subsequent years.

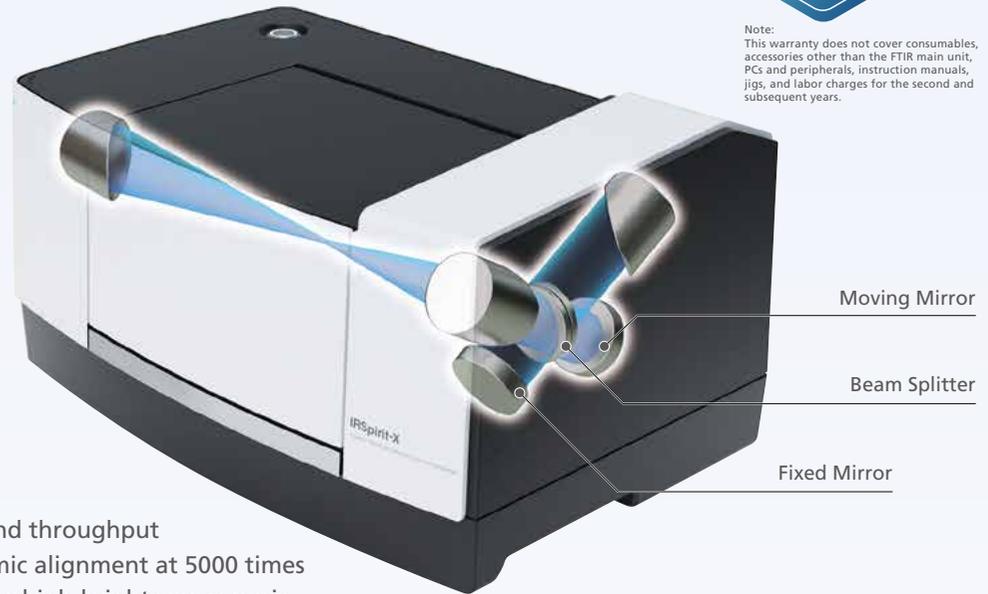

- High stability and throughput (Features dynamic alignment at 5000 times per second and a high-brightness ceramic light source)
- High sensitivity comparable to standard models (IRSpirit-TX) (DLATGS detector with temperature control function)

The silicone oil content in paraffin oil (1.0%) was obtained by repeating a single-reflection ATR method five times. Data obtained using the DLATGS detector with temperature control is shown on the left and data obtained using the DLATGS detector without temperature control is shown on the right. The internal heat in the instrument and the environmental temperature caused large baseline data fluctuations without temperature control. In contrast, using the detector with temperature control resulted in highly repeatable data.

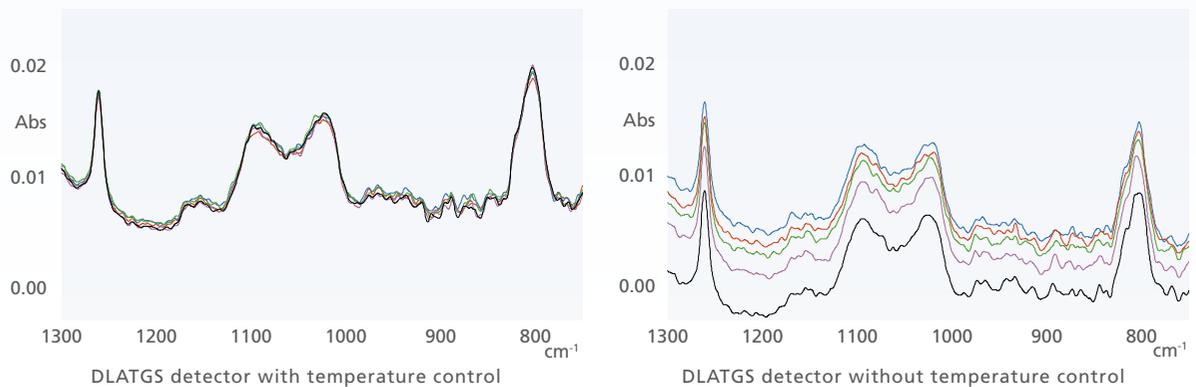

ATR Spectra of Silicone Oil Content in Paraffin Oil (measurement repeated five times)

## High Durability Due to Humidity-Resistant Design

The robust optics are designed to ensure the system can be used reliably even under harsh temperature and humidity conditions.

- KBr beam splitter includes a humidity-resistant coating (IRSpirit-TX/LX), or ZnSe beam splitter (IRSpirit-ZX)<sup>\*1</sup>
- Optics sealed in an aluminum die cast housing
- Status monitor function features electrical and paper-based indicators.
- Select from a KBr window (to 70% RH) or a KRS-5 window (to 90% RH); both include a humidity-resistant coating.<sup>\*2, \*3</sup>
- Optional electric dehumidifier can be installed.<sup>\*4</sup>



Aluminum Die Cast Interferometer Housing


\*1 The measurement wavenumber range will be 6,000 to 550  $\text{cm}^{-1}$  with the IRSpirit-ZX, which is equipped with a ZnSe beam splitter.

\*2 No condensation

\*3 The KRS-5 window plate is used with the IRSpirit-ZX.

\*4 Not required with the IRSpirit-ZX.


Window		
Humidity Resistance	With humidity-resistant coating Max. humidity at installation site: 70 %RH (with no condensation)	Max. humidity at installation site: 90 %RH (provided no condensation at temperatures up to 30 °C)
Wavenumber Range	350 to 7,800 $\text{cm}^{-1}$	
Transmittance	About 90 %T	About 70 %T
Characteristics	<ul style="list-style-type: none"> <li>• High transmittance and high sensitivity</li> <li>• Could deliquesce in humid environments</li> </ul>	Compared to KBr window: <ul style="list-style-type: none"> <li>• Higher humidity-resistance</li> <li>• Lower S/N due to lower transmittance</li> </ul>

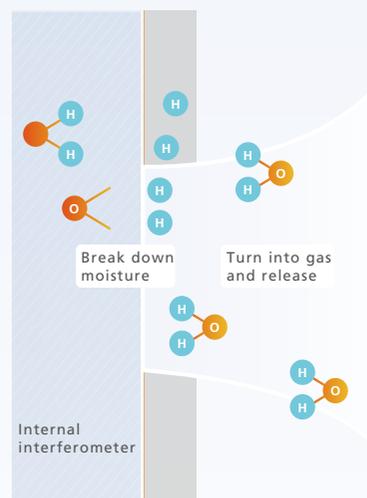

The Principle of a Dehumidifier

## Internal Dehumidifier (Optional) Ensures Robustness

This dehumidifier removes moisture from inside the interferometer electrolytically using a solid polymer electrolytic membrane. It maintains low humidity levels inside the interferometer without leaving the light source ON. Using the dehumidifier alone can reduce power consumption by about 90 % compared to leaving the light source illuminated. Note that a dehumidifier is not required as the ZnSe beam splitter adopted for the IRSpirit-ZX features high resistance to humidity.

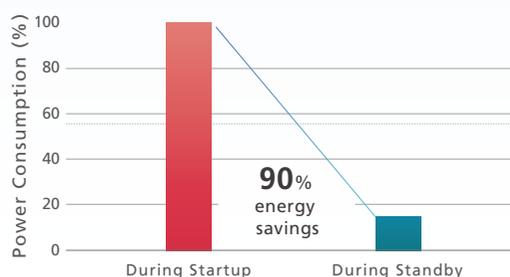

IRSpirit-X series power consumption during Startup (with Start Switch ON) and during Standby (with Start Switch OFF and Dehumidifier ON)

## Instrument Status Monitoring

Instrument status is automatically verified during start-up and results are saved in a report. This feature is especially convenient for instrument management. Pharmacopoeia-compliant validation programs convenient for routine inspections are also included.

### Self-diagnostic function

A self-diagnostic function inspects the signal system and optics during instrument initialization. It obtains a variety of information and automatically outputs the results in one file, making instrument management easy.

The instrument status history can also be confirmed.



### Status monitor function


This function continuously monitors and manages information about the light source, semiconductor laser, humidity inside the instrument, the window plate connection (interlock), and accessories.



## Simple Operation, Confident Results

LabSolutions™ IR automates routine work, such as scanning, data manipulation, reporting, identification tests, and contaminants analysis. Launch programs from the Launcher or your PC.

### Easy Macro – Just a Single Click Launches Routine Work

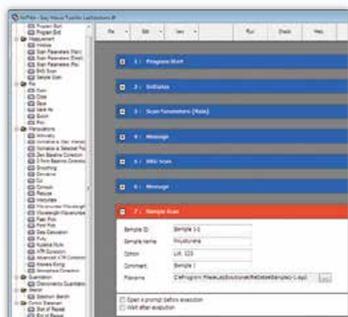

- ✓ Initialization of FTIR, configuration of scan parameters, spectrum measurement
- ✓ Data manipulations, search, quantitation, printing
- ✓ Repeat measurements, displaying messages, alarm sounds, external program execution

The “Easy Macro” function will create macros that are suitable for routine work, particularly when repetitive operations are used. The macro builder allows macros to be constructed by simply selecting and aligning operations from a list. Once constructed, the macros can be registered with the Launcher and Desktop for quick execution. Operators who are not familiar with FTIR can easily operate the instrument.

# Acquisition and Analysis of EDX and FTIR Data from a Single Computer

Both EDX and FTIR models can be controlled with a single computer. The efficiency of time-consuming contaminant analysis can be improved by installing EDXIR-Analysis™, an integrated EDX/FTIR analysis program, on the computer.

## Integrated Data Analysis for Contaminants


- ✓ To perform qualitative analysis automatically, simply click "Analyze Both Data" and select the EDX/FTIR data.\*1
- ✓ This enhances the efficiency of time-consuming analyses that were traditionally left to the analyst, and provides strong support for contaminant analysis.
- ✓ In addition to a list of hits, the integrated data analysis results show EDX profiles and FTIR spectra found as hits from the library.

## Data Comparisons for Identification Tests

- ✓ A Data Comparison function calculates the degree of matching between the actual measured data and the data registered in the library.
- ✓ The software can be used for countermeasures against "silent change" and for other confirmation tests.
- ✓ Clicking the "Print" button prints the results in a fixed format and also saves them in Word format.\*2

\*1 Using the EDX profile, data are classified as organic, inorganic, and mixture. Integrated data analysis is performed by applying priority levels to each classification (Patent No. 06638537).

\*2 Microsoft® Word must be installed.

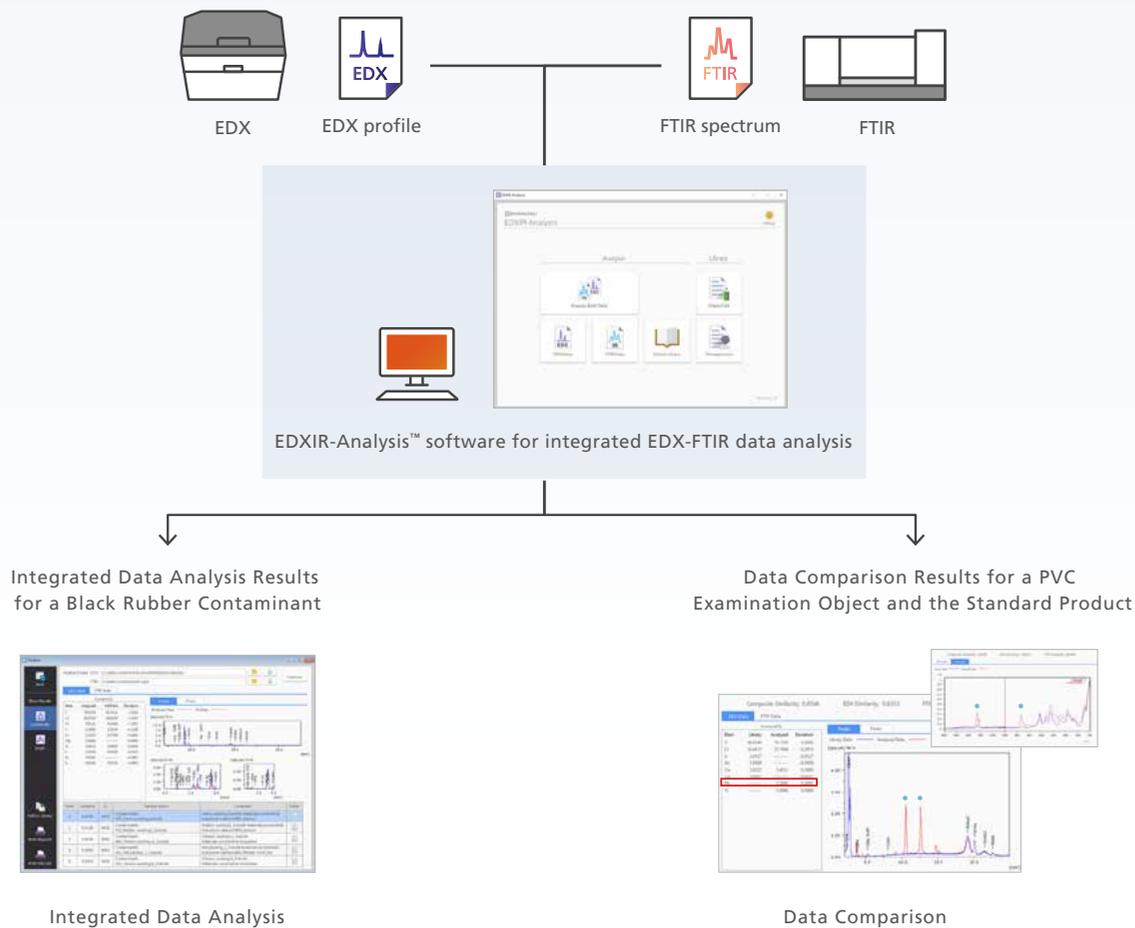

## Reliable LabSolutions™ Software

In addition to LabSolutions IR, which provides basic functionality, Shimadzu also offers LabSolutions DB IR and LabSolutions CS IR to meet the requirements of ER/ES regulations.


### LabSolutions DB IR

LabSolutions DB IR allows for secure data management by integrating a data management function with LabSolutions IR. Compliant with ER/ES regulations, the software is optimally configured for customers using a PC. It is recommended for facilities that do not require network connections and want to be ER/ES compliant.




### LabSolutions CS IR

Since all the data are managed on a server, LabSolutions CS IR, which is freely accessible to the analysis network, can be connected to IR and can be read from any personal computer on the network. It is recommended for facilities that have many users, manage data in a database, and want to be ER/ES compliant.

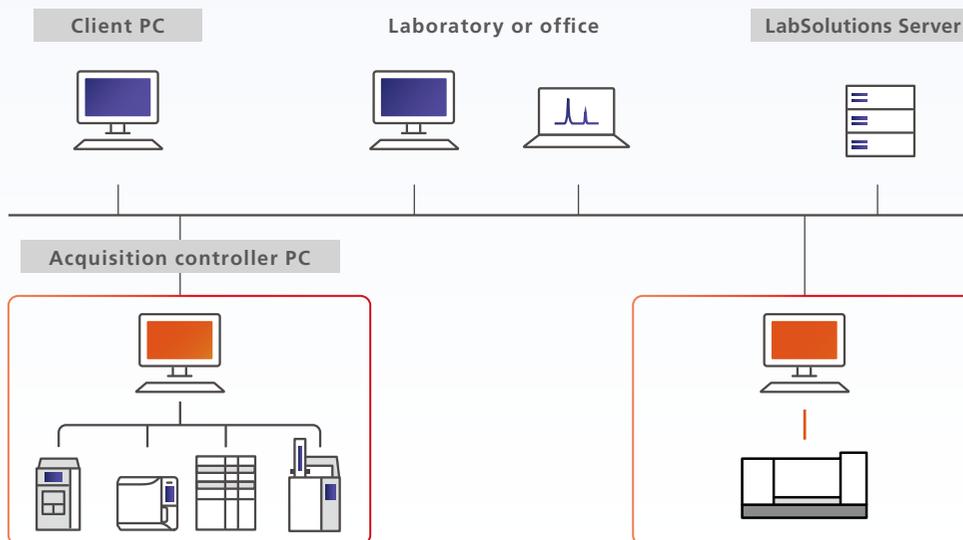

## Data Integrity Compliance

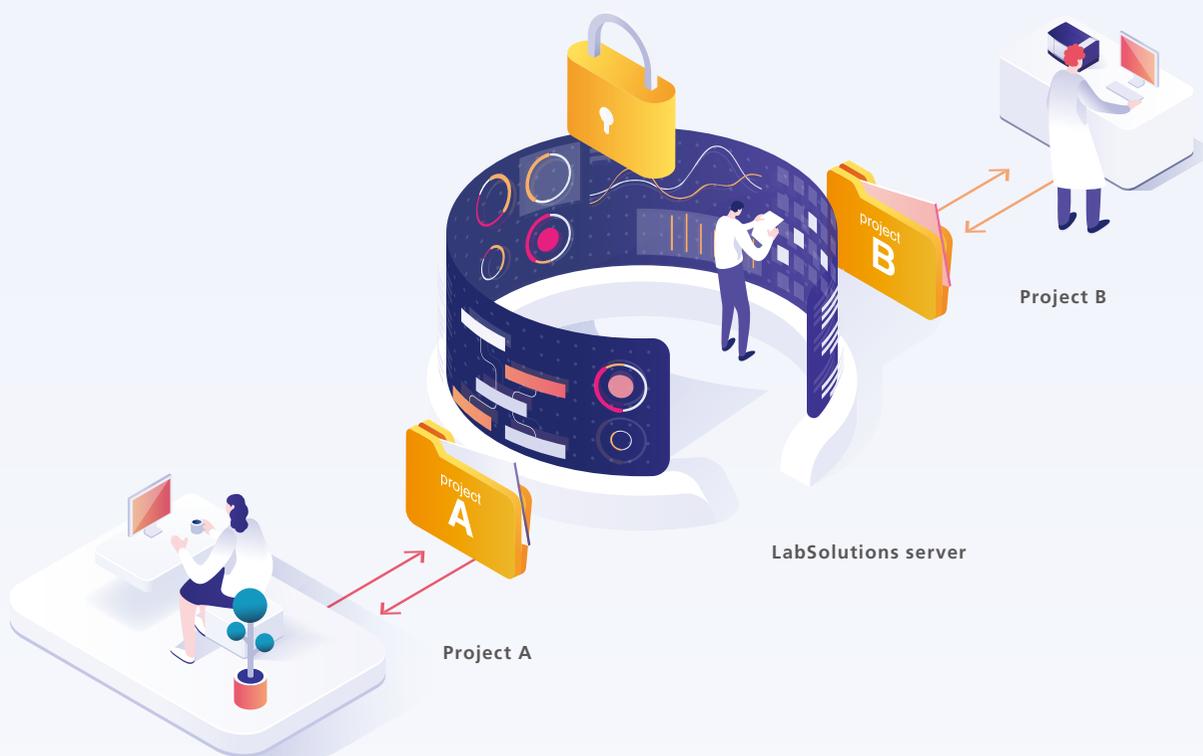

### High Security

An audit trail to ensure the reliability of data and document e-mail transmission functions when any event occurs in the system can be set up. User accounts are managed using passwords, where password length, complexity and term of validity must satisfy specified requirements. It is also possible to set lockout functions to prevent illegal access, and set a registered user's deletion and change in status. In addition, a box can be selected to prevent overwriting a data file and outputting an item to a report.

### Essential Information Is Managed for Every Project

LabSolutions DB IR and CS IR provide a project management function enabling control suited to tasks and system operations. This function enables equipment and user management, security policy, and data processing to be set on a project by project basis, thereby improving the efficiency of data searches and management tasks.

### Visualization of the Sequence of Analysis Operations

Report set includes test methods and test results for a series of samples analyzed as well as a corresponding operation log (a record of all operating events from login to logout), which is automatically extracted from the data and summarized in a single report. It provides visibility of the individual analytical operations, and helps to check for operating errors and improve the efficiency and reliability of checking processes.

## Hardware/Software



### Pharmaceutical

#### MHP-1

This is a compact, inexpensive hand-driven press used to produce 4 mm dia KBr pellets. A pellet produced in the frame is directly measured using the dedicated holder, which ensures exceptional simplicity of operation. No dies or a vacuum pump are required. (Samples That Can Be Measured: Powders)



#### DRS-8000A

Although powder samples are mixed with KBr, as with the KBr pellet method, the DRS-8000A analyzes the samples in their original state; creating pellets is not necessary. For plastic moldings, emery paper attached to the SiC sampler (P/N 200-66750-01) scrapes off part of the surface, forming a powdered sample that can be analyzed. Easily obtain diffuse reflectance spectra similar to transmittance spectra using the built-in Kubelka-Munk conversion function in LabSolutions IR software. Functionality is included for automatically recognizing attached accessories. (Samples That Can Be Measured: Powders, Moldings)



### Polymer/Materials

#### QATR™-S

This is a single reflection ATR measurement attachment. The prism is made entirely of diamond, so the measurement wavenumber range is up to 400  $\text{cm}^{-1}$  (wide-band). With a liquid sample, simply place a drop on the prism to measure spectra. For other samples, clamp the sample closely against the prism surface before measurement on the sample surface. The incident angle is 45 degrees. Four prism materials are available: diamond, (wide-band, high-throughput), germanium (Ge) or zinc selenide (ZnSe). The Ge prism is best suited for samples with a high refractive index.



#### Dehumidifier Unit

This is the same electric dehumidifier unit used in our higher-end models (IRXross™ and IRTracer™-100). The dehumidifier is driven by a stand-by power, so it is possible to maintain a low level of humidity inside the interferometer even when the FTIR is not used (AC power supply). It can reduce the labor and maintenance costs associated with replacing the silica gel.

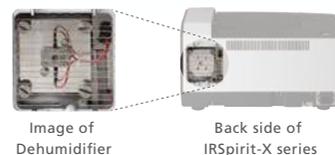



Image of Dehumidifier

Back side of IRSpirit-X series

## Contaminant Library for LabSolutions IR

This is Shimadzu's latest original library. It is an effective tool for analyzing contaminants in tap water and food. In addition to containing information on actual sample contaminants and information about water supply maintenance parts commercially available in Japan, the library also includes X-ray fluorescence profiles (PDF files) to significantly improve the accuracy of contaminant searches. Unlike existing libraries, this library contains data on mixed compounds and incorporates the depth of knowledge and experience needed to make qualitative assessments.

## EDXIR-Analysis™ Software

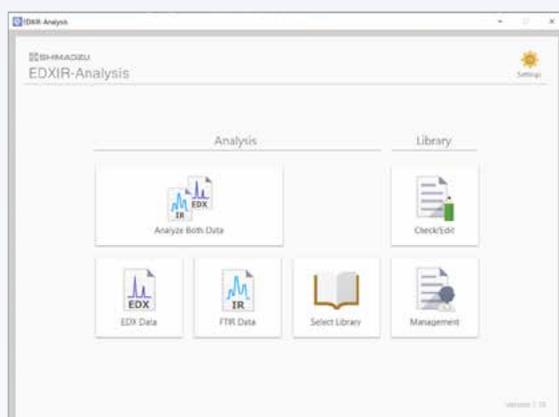

EDXIR-Analysis software is specially designed to perform qualitative analysis using data acquired by an energy dispersive X-ray (EDX) fluorescence spectrometer and a Fourier transform infrared (FTIR) spectrophotometer. This software is used to perform an integrated analysis of data from FTIR, which is excellent at the identification and qualification of organic compounds, and from EDX, which is excellent at the elementary analysis of metals, inorganic compounds and other content. It then pursues identification results and the degree of matching. It can also be used to perform EDX or FTIR data analysis individually. The library used for data analysis (containing 485 data files) is original to Shimadzu, and was created through cooperation with water supply agencies and food manufacturers. Additional data can be registered to the library, as can image files and document files in PDF format. It is also effective for the linked storage of various types of data as electronic files.

## EDXIR-Holder™



Image of measurement with EDX



Image of measurement with FTIR

This foldable holder consists of an adhesive layer with samples attached and polypropylene film designed for X-ray fluorescence analysis.

It provides measurement by keeping the samples in the holder with EDX and FTIR.


When using EDX for measurement, close the holder and place the polypropylene film directly to the irradiation side (downside). When using FTIR for measurement, open the holder and press the samples attached to the adhesive layer against the ATR prism. Close the holder after the measurement and it can be used as sample storage.



## Semiconductor

### Time Course Software

The time course program is used to collect spectra in regular intervals and creates a time course dataset used to follow reactions as a function of time. Changes in peak height and peak area can be used to calculate values related to reaction kinetics. Time course information is saved and displayed in 3D or in a contour plot.

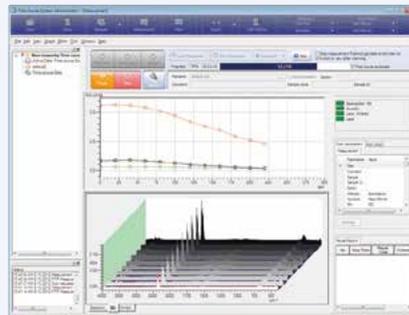

## Environmental

### Plastic Analyzer

#### Configurations

- Fourier transform infrared spectrophotometer
- Single-reflection ATR attachment
- Plastic Analyzer method package
  1. UV-Damaged Plastics Library
  2. Thermal-Damaged Plastics Library
  3. Macro Program for IR Pilot/Parameter File



When analyzing plastics, libraries are used to qualify their material properties. However, infrared spectra of plastics that have degraded due to heat or UV rays differ in shape from standard spectra, and qualifying them can sometimes be difficult. To address this, the Plastic Analyzer includes a deterioration library, so highly accurate qualification can be performed reflecting the state of deterioration.

### Thermal-Damaged Plastics Library\*<sup>1</sup> / UV-Damaged Plastics Library\*<sup>2</sup>


These libraries contain plastic samples which have oxidized and degraded due to UV rays and heat. They are designed to be effective when searching for deteriorated materials, making it useful in cases where degradation has occurred. The target materials for search often include degraded ones, making these libraries effective for analyzing such materials.

\*<sup>1</sup> Shimadzu created the library using spectra obtained by Hamamatsu Technical Support Center, Industrial Research Institute of Shizuoka Prefecture.


\*<sup>2</sup> Plastics which were degraded for 10 years by using an Iwasaki Electric super accelerated weathering tester were measured and compiled as a library by Shimadzu Corporation.

# Analysis Example with Plastic Analyzer

## Evaluation of Deteriorated Samples

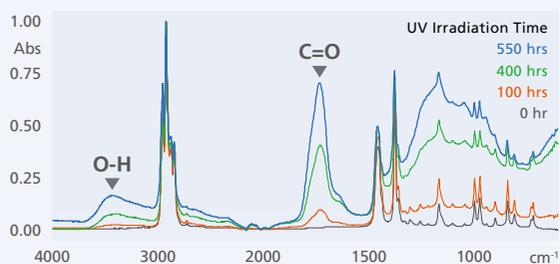


Plastics degrade as they experience molecular cleavage and cross-linking due to heat and light. As a result, in fault analysis and failure analysis, the qualities of deteriorated samples must be analyzed. The above left figure shows the infrared spectrum of a polypropylene (PP) sample that has been irradiated with UV rays. The UV irradiation has caused the plastic to deteriorate, and it is evident that the shape of the infrared spectrum has changed.

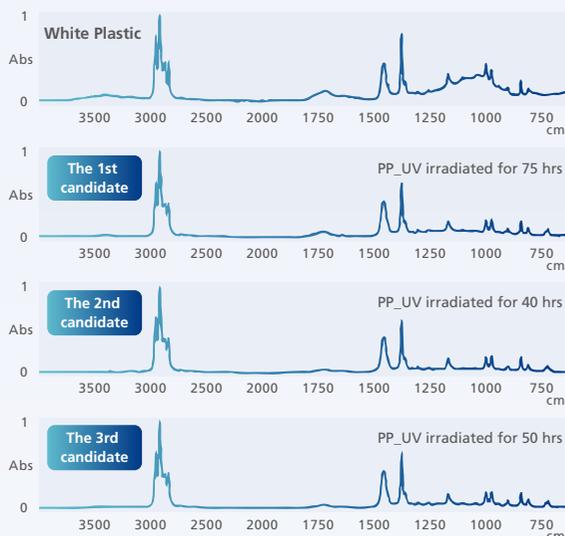


The top right figure shows the search results from measurements by Plastic Analyzer of a white plastic (PP material) that was left outdoors for an extended period and exposed to UV rays.

The infrared spectrum of the sample exposed to UV rays differs from the standard spectrum. Accordingly, in general library searches, different plastics such as polybutene are at the top of the results. In contrast, with Plastic Analyzer, PP denatured by UV rays is the top result.

## Contaminant Analysis (Contaminants in Processed Items)

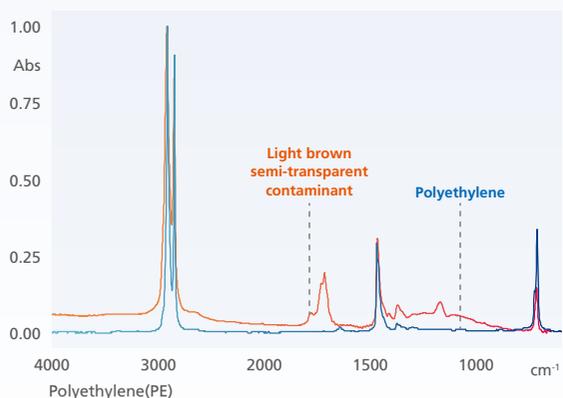

A light brown semi-transparent contaminant on a plated item

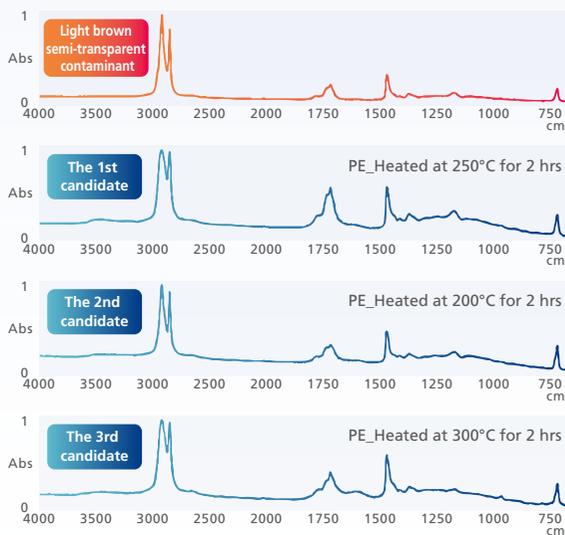

The measurement of a light brown semi-transparent contaminant on a plated item was performed. The figure above shows that the spectral pattern of the acquired infrared spectrum differs from the standard polyethylene (PE).

Plastic Analyzer shows the best match is heated PE. The Thermal-Damaged Library makes it useful for surmising the thermal history of the plastic.





## Transporting and Moving the Instrument

When transporting and moving the instrument, avoid vibrations, falls, or other strong impacts. When transporting it over long distances, such as to another building, use the original packaging. Note that Shimadzu is not responsible for performance deterioration resulting from transportation or movement of the instrument.



- Automated support functions utilizing digital technologies, such as M2M, IoT, and Artificial Intelligence (AI), that enable higher productivity and maximum reliability.
- Allows a system to monitor and diagnose itself, handle any issues during data acquisition without user input, and automatically behave as if it were operated by an expert.
- Supports the acquisition of high quality, reproducible data regardless of an operator's skill level for both routine and demanding applications.



This product is certified as Shimadzu's Eco-products Plus.

Energy savings: 62% reduction as compared to the conventional model\*

Space savings: 76% reduction of weight as compared to the conventional model\*

70% reduction of installation area as compared to the conventional model\*

\*: The comparison with our conventional model.

IRSpirit, IR Pilot, IRXross, IRTracer, LabSolutions, QATR, EDXIR-Holder, EDXIR-Analysis, Analytical Intelligence logo and eco mark are trademarks of Shimadzu Corporation or its affiliated companies in Japan and/or other countries.

Microsoft is either a registered trademark or a trademark of Microsoft Corporation in the United States and/or other countries.



Shimadzu Corporation

[www.shimadzu.com/an/](http://www.shimadzu.com/an/)

### For Research Use Only. Not for use in diagnostic procedures.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

Company names, products/service names and logos used in this publication are trademarks and trade names of Shimadzu Corporation, its subsidiaries or its affiliates, whether or not they are used with trademark symbol "TM" or "®".

Third-party trademarks and trade names may be used in this publication to refer to either the entities or their products/services, whether or not they are used with trademark symbol "TM" or "®".

Shimadzu disclaims any proprietary interest in trademarks and trade names other than its own.

The contents of this publication are provided to you "as is" without warranty of any kind, and are subject to change without notice. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication.