

Analysis of Acrylamide in Potato Chips by SPE and GC-MS

Anila I. Khan, Thermo Fisher Scientific, Runcorn, UK

Key Words

Hypercarb SPE, food, acrylamide, 2-propenamide, capillary GC, porous graphitic carbon (PGC), polyethylene glycol (PEG) GC column

Abstract

Acrylamide is an endogenous compound, formed when heating starchy or sugary foods. The production of potato chips can result in its formation. The method reported here detects acrylamide at the low ng/g levels at which it is produced. Potato chips were extracted using porous graphitic carbon for solid phase extraction (SPE). Analysis of acrylamide was performed using GC-MS on a polyethylene glycol phase GC column. A standard addition calibration curve was used to estimate the level of acrylamide in potato chips at 450 ng/g.

Introduction

Acrylamide (2-propenamide) is a potential human carcinogen. This toxic compound is usually formed as a by-product of Maillard reactions during the heating of carbohydrate-rich food. The World Health Organization (WHO) has set a safe limit of 500 ng/mL acrylamide in drinking water. Higher levels of 100–1000 ng/g are determined in some foods such as potato chips or french fries.

The extraction of acrylamide from potato chips is carried out using a Thermo Scientific™ HyperSep™ Hypercarb™ SPE cartridge. Hypercarb SPE material is 100% porous graphitic carbon (PGC) and offers retention of highly polar compounds that are not usually retained by traditional reversed phase C18 columns. HyperSep Hypercarb SPE can produce clean samples by removing potential matrix interferences.

The analysis of acrylamide was carried out using a GC-MS in electron ionization (EI) mode. Quantitative measurement in food can be difficult as matrix-derived ions can interfere with acrylamide fragment ions of m/z 71, 55, and 41 when using this mode. Acrylamide often requires derivatization to improve sensitivity on a mass spectrometer. In this case, acrylamide is injected without derivatization onto a Thermo Scientific™ DSQ™ II mass spectrometer and an ultra low bleed Thermo Scientific™ TraceGOLD™ TG-WaxMS™ 30 m × 0.25 mm × 0.25 μm GC column.



Acrylamide is a highly polar water soluble compound having a logP value of -0.65 [1]. Such highly polar compounds are not readily amenable to GC, therefore a polar GC column is required. The TraceGOLD TG-WaxMS column is a polyethylene glycol-phase GC column that allows the analysis of polar compounds.

Experimental Details

Consumables		Part Number
Cartridge type:	HyperSep Hypercarb SPE cartridge, 500 mg/6 mL	60106-402
Column:	TraceGOLD TG-WaxMS, 30 m × 0.25 mm × 0.25 µm	26088-1420
Septum:	Thermo Scientific BTO, 17 mm	31303211
Liner:	Thermo Scientific™ Splitless FocusLiner™, 3 × 8 × 105 mm	45354032
Column ferrules:	100% graphite ferrules for Thermo Scientific™ TRACE™ injector, 0.1–0.25 mm i.d.	29053488
Column ferrules:	Graphite/Vespel® for transfer line 0.1–0.25 mm i.d.	29033496
Vials and closures:	Thermo Scientific™ Chromacol™ 9 mm screw, 2 mL vial, amber	2-SVW(A)
	Chromacol 9 mm screw caps with silicone/PTFE septa 9-SC(B)-ST101	
Syringe filter:	Thermo Scientific™ Target2™ 30 mm GMF syringe filter membrane, 3.1 µm pore size	F2500-20
Plastic syringe:	Thermo Scientific 3 mL plastic disposable syringes	S7510-3

Sample Handling Equipment		Part Number
HyperSep glass block manifold		60104-232

Instrumentation

Thermo Scientific™ TRACE GC Ultra™ gas chromatograph
 Thermo Scientific™ DSQ™ II single quadrupole mass spectrometer
 Thermo Scientific™ TriPlus™ Autosampler

Chemicals and Reagents		Part Number
Fisher Scientific™ HPLC grade water		W/0106/17
Fisher Scientific HPLC grade methanol		M/4056/17
Fisher Scientific Analytical grade formic acid		F/1900/PB08

Sample Pretreatment

The potato chips were finely crushed with mortar and pestle and 1 g was weighed into a vial. A 1 g portion of the sample was spiked with 25, 50, 100, 250, 500, and 1000 ng/g of acrylamide standard in 2% formic acid / water. The sample was then filtered through a filter membrane.

Sample Preparation

Compounds:	Acrylamide and acrylamide-d ₃ (internal standard)
Matrix:	Potato chips
Conditioning stage:	Add 4 mL methanol, 4 mL water, and 4 mL 2% formic acid / water to the SPE cartridge.
Application stage:	Apply 1 mL of extract in 2% formic acid / water under vacuum at 1 mL/min to the SPE cartridge.
Washing stage:	Add 1 mL water to the SPE cartridge and dry for 20 min under vacuum.
Elution stage:	Apply 4 mL methanol to the SPE cartridge.
Additional stage:	Evaporate methanolic extract and reconstitute with 1 mL of 1 µg/mL of internal standard in methanol to the SPE cartridge.

Separation Conditions

Carrier gas:	Helium
Split flow:	50 mL/min
Column flow:	1.2 mL/min, constant flow
Oven temperature:	80 °C, 10 °C/min, 250 °C
Injector type:	Split/Splitless
Injector mode:	Splitless (1 min), constant septum purge
Injector temperature:	230 °C

Instrumentation

Transfer line temperature:	150 °C
Source temperature:	200 °C
Ionization conditions:	EI
Electron energy:	70 eV
SIM scan parameters:	m/z 71 for acrylamide and m/z 74 for acrylamide- d_3
Start time:	4.0 min
Dwell time:	0.1 s

Injection Conditions

Injection volume:	2 μ L
Pre- and post-needle injection dwell time:	0.5 s

Data Processing

Software:	Thermo Scientific™ Xcalibur™ software
-----------	---------------------------------------

Results

A standard addition calibration curve was constructed for acrylamide in matrix over the range 25–1000 ng/g. Standard addition calibration was chosen because acrylamide is endogenous in cooked foods and a suitable blank matrix was unavailable.

The amount of acrylamide present in the potato chips was calculated to be 450 ng/g. The chromatogram in Figure 1 shows the acrylamide peak in potato chips and acrylamide- d_3 internal standard spiked in potato chips.

The acrylamide concentration was calculated using the integrated response ratio of acrylamide/ acrylamide- d_3 (m/z 71/74). The acrylamide in the potato chips was calculated from the intercept of the x axis. An excellent linearity was demonstrated for this method with a coefficient of determination (R^2) of 0.999.

The accuracy of the back calculated concentrations for the amount of acrylamide spiked in potato chips was less than 10% (see Table 1).

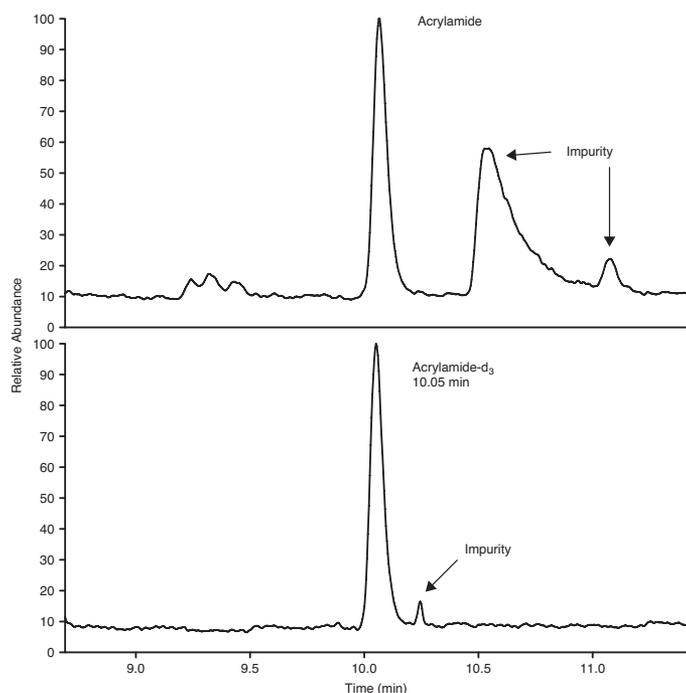


Figure 1: TIC of chromatogram of 1 µg/mL spiked acrylamide (m/z 71) and acrylamide- d_3 (m/z 74) extracted from potato chips

Specified Concentration (µg/mL)	Calculated Concentration	% Difference
0.25	0.225	-9.83
0.50	0.469	-6.22
1.00	0.983	-1.70
2.50	2.520	0.79
5.00	4.979	-0.41
10.0	10.037	0.37

Table 1: Accuracy data for the standard addition calibration curve for spiked acrylamide in potato chips

Conclusion

HyperSep Hypercarb SPE cartridges offer high levels of reproducibility as well as cleaner extracts, which yields very good results. TraceGOLD TG-WaxMS GC columns are suitable for the GC-MS analysis of acrylamide because of the low bleed stationary phase and better retention of polar analytes compared with lower polarity stationary phases.

Reference

- [1] Acrylamide in Drinking-water - Background document for development of WHO Guidelines for Drinking-water, 2011, http://www.who.int/water_sanitation_health/dwq/chemicals/acrylamide.pdf

thermoscientific.com/columnsforge

© 2013 Thermo Fisher Scientific Inc. All rights reserved. Vespel is a registered trademark of E. I. du Pont de Nemours and Company. All other trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. This information is presented as an example of the capabilities of Thermo Fisher Scientific Inc. products. It is not intended to encourage use of these products in any manners that might infringe the intellectual property rights of others. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

USA and Canada +1 800 332 3331
France +33 (0)1 60 92 48 34
Germany +49 (0) 2423 9431 20 or 21
United Kingdom +44 (0)1928 534110
Japan +81 3 5826 1615

China +86 21 68654588 +86 10 84193588
 +86 20 83145199 800 810 5118
India +91 22 6742 9494 +91 27 1766 2352
Australia 1 300 735 292 (free call domestic)
New Zealand 0800 933 966 (free call domestic)
All Other Enquiries +44 (0) 1928 534 050

Technical Support
North America +1 800 332 3331
Outside North America +44 (0) 1928 534 440

Thermo
 SCIENTIFIC

Part of Thermo Fisher Scientific