



307 Lewers St., Suite 707  
Honolulu, HI 96815  
1-888-387-6344



## Certificate of Calibration

Date: May 5, 2025

Cert No. [REDACTED]

Customer: [REDACTED]

[REDACTED]

MPC Control #: [REDACTED]

Asset ID: N/A

Gage Type: DRY BATH

Manufacturer: THERMO SCIENTIFIC

Model Number: 88870001

Size: 36.5 DEG C

Temp/RH: 20.0°C / 40.0%

Location: Calibration performed at Customer's facility

Work Order #: [REDACTED]

Purchase Order #: [REDACTED]

Serial Number: [REDACTED]

Department: N/A

Performed By: GLENN HIGGINS

Received Condition: IN TOLERANCE

Returned Condition: IN TOLERANCE

Cal. Date: April 29, 2025

Cal. Interval: 12 MONTHS

Cal. Due Date: April 29, 2026

### Calibration Notes:

SEE ATTACHED DATA

### Standards Used to Calibrate Equipment

I.D.	Description.	Model	Serial	Manufacturer	Cal. Due Date	Traceability #
[REDACTED]	DOCUMENTING PROCESS CALIBRATOR	744	[REDACTED]	FLUKE	Nov 30, 2025	[REDACTED]

### Procedures Used In this Event

Procedure Name	Description
MPC-00074 Rev. 02	Temperature Devices, Sept-27-2016 rev02

Calibrating Technician:

  
GLENN HIGGINS

QC Approval:

  
ROBERT MEANS

**STATEMENTS OF PASS OR FAIL CONFORMANCE:** The uncertainty of measurement has been taken into account when determining conformance with specification. All measurements and test results guard banded to ensure the probability of false-accept does not exceed 2% in conformance with ANSI/NCSL Z540.3-2006

**THE CALIBRATION REPORT STATUS:**

PASS - Term used when conformance statement is given and the measurement result is PASS.

PASS<sup>2</sup> - Term used when conformance statement is given and the measurement result is conditionally passed or PASS<sup>2</sup>.

FAIL - Term used when conformance statement is given and the measurement result is FAIL.

FAIL<sup>2</sup> - Term used when conformance statement is given and the measurement result is conditionally failed or FAIL<sup>2</sup>.

**REPORT OF VALUE** - Term used when reported measurement is not requiring conformance statement in report.

**ADJUSTED** - When adjustments are made to an instrument which changes the value of measurement from what was measured as found to new value as adjusted.

**LIMITED** - When an instrument fails a calibration but still functions in a limited manner.

The expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2 which for a normal distribution corresponds to a coverage probability of approximately 95% unless otherwise stated. This calibration report complies with ISO/IEC 17025:2017 ANSI/NCSL Z540.3-2006 and ANSI/NCSL Z540.1-1994. Calibration cycles and resulting due dates were submitted/approved by the customer. Any number of factors may cause an instrument to drift out of tolerance before the next scheduled calibration. Recalibration cycles should be based on frequency of use, environmental conditions and customer's established systematic accuracy. All standards are traceable to SI through the National Institute of Standards and Technology (NIST) and/or recognized national or international standards laboratories. Services rendered include proper manufacturer's service instruction and are warranted for no less than thirty (30) days. The information on this report pertains only to the instrument identified. This may not be reproduced in part or in whole without the prior written approval of the issuing MP Calibration Laboratory.

## Calibration Report of Fisher Scientific 88870001 Dry Bath

MPC Control #:	[REDACTED]	Serial Number:	[REDACTED]
Asset ID:	[REDACTED]	Calibration Date:	April 29, 2025

### Temperature Accuracy


Range	Nominal	Lower Limit	As Found	As Left	Upper Limit	Result
36.5 Deg C	36.5 °C	36.0 °C	36.2 °C	36.2 °C	37.0 °C	PASS

### Statements of Pass or Fail Conformance

The status of compliance with the acceptance criteria is reported as:

PASS — Compliant with specification.

FAIL — Not compliant with specification.

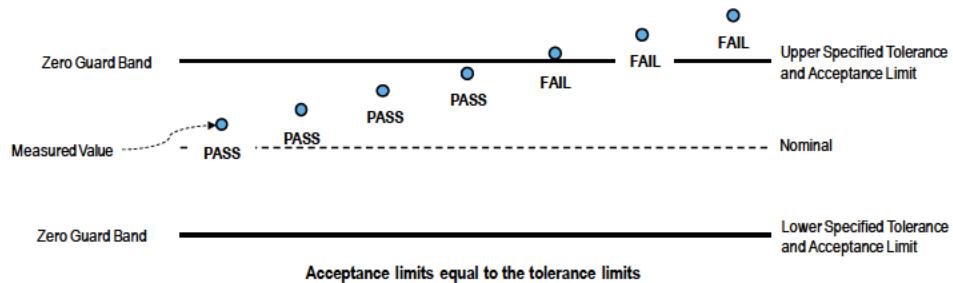

- End of Calibration Report -