


**Figure S23**


**A**

parameter	value
1 Cytokine	MCP-1
2 Vendor	Bio-Rad
3 Samples included in this agreement	15
4 Proportion of both readings in range	40.5
5 Limits of agreement	0.73 to 1.45
6 Constant variance p.value	0.488
7 Constant ratio p.value	0.103
8 Ratio is 1 p.value	0.483

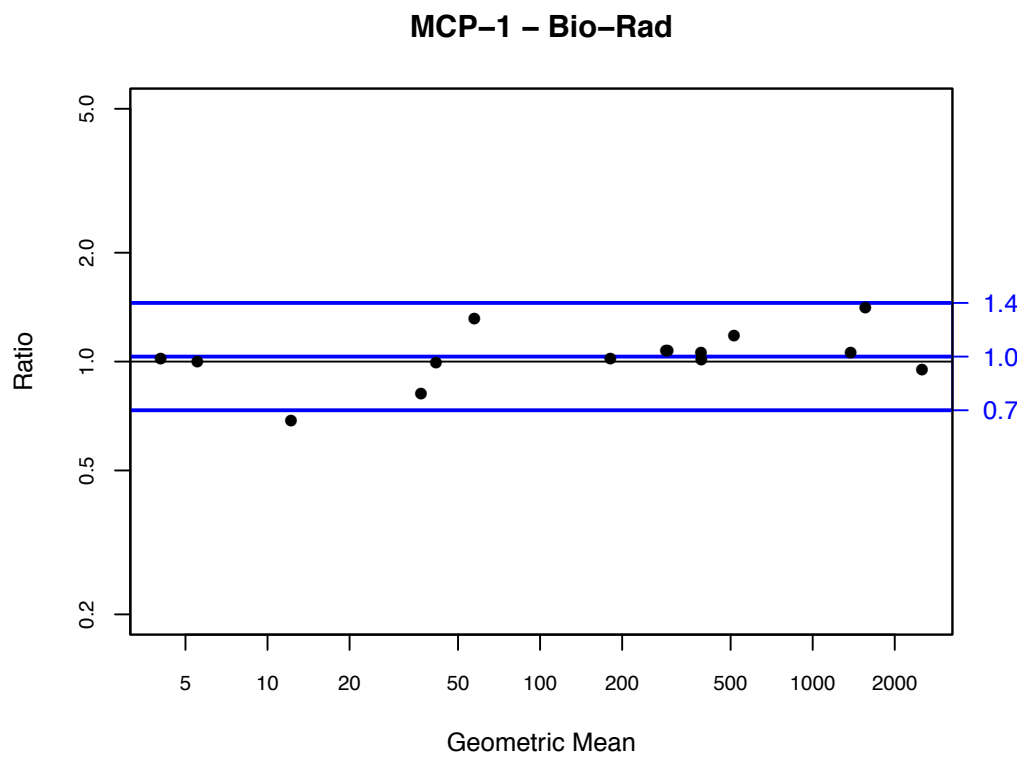

**B**

parameter	value
1 Cytokine	MCP-1
2 Vendor	Invitrogen
3 Samples included in this agreement	21
4 Proportion of both readings in range	56.8
5 Limits of agreement	0.39 to 2.30
6 Constant variance p.value	0.829
7 Constant ratio p.value	0.532
8 Ratio is 1 p.value	0.608

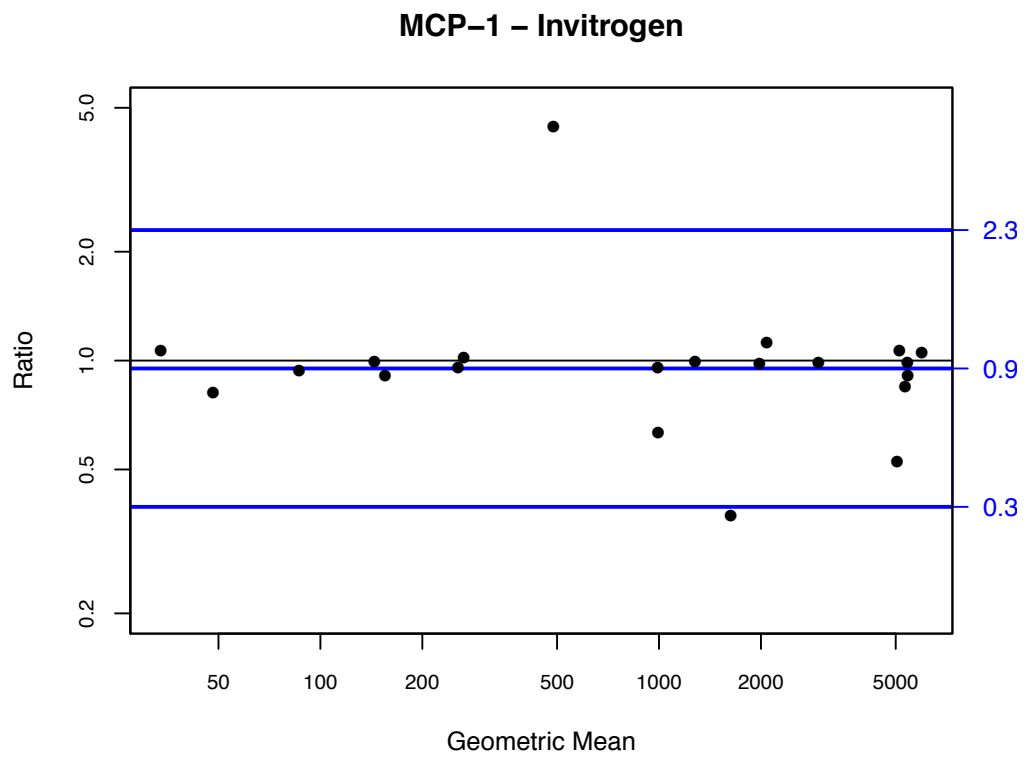

C

parameter	value
1 Cytokine	MCP-1
2 Vendor	INV_MAG
3 Samples included in this agreement	24
4 Proportion of both readings in range	60.0
5 Limits of agreement	0.81 to 1.28
6 Constant variance p.value	0.251
7 Constant ratio p.value	0.371
8 Ratio is 1 p.value	0.384

