

User Manual

Trinocular Compound PLAN Microscope

Model M834PLAN Series



MicroscopeNet.com

Table of Contents

| | |
|---|----|
| i. Caution..... | 1 |
| ii. Care and Maintenance..... | 2 |
| 1. Component Illustration..... | 3 |
| 2. Installation | 4 |
| 3. Operation..... | 7 |
| 4. Specifications..... | 10 |
| 5. Optional Parts..... | 11 |
| 6. Troubleshooting Guide..... | 13 |
| 7. Darkfield Condenser Installation and Operation Instructions..... | 15 |
| 8. Phase Contrast Kit Installation and Operation Instructions..... | 16 |


i. Caution

1. Find the “UP” sign and place the Styrofoam container on your table or bench so that the arrow is pointing upward. Open the shipping carton carefully to prevent any accessory items (i.e. objectives or eyepieces) from dropping and being damaged.
2. Do not discard the molded Styrofoam container. The container should be retained should the microscope ever requires reshipment.
3. Keep the instrument out of direct sunlight, high temperature or humidity, and dusty environments. Ensure that the microscope is located on a smooth, level and firm surface.
4. If any specimen solutions or other liquids splash onto the stage, objective or any other component, disconnect the power cord immediately and wipe up the spillage. Otherwise, the instrument may be damaged.
5. All electrical connectors (power cord) should be inserted into an electrical surge suppressor to prevent damage due to voltage fluctuations.
6. **Important:** the lamp, lamphouse and adjacent parts will become very hot during or short after operation. Do not touch these parts until they have completely cooled. Never attempt to handle a hot halogen bulb or mercury bulb.
7. Make sure there is sufficient room around the microscope base for heat elimination.
8. For safety when replacing the lamps or fuses, be sure the main switch is off, unplug the power cord, and only replace the bulb after the bulb and the lamphouse has completely cooled.
9. Do not touch the surface of halogen bulbs with bare fingers. If so, clean the surface with soft cloth.
10. **Important:** confirm that the input voltage (**220V version available, contact seller**) indicated on your microscope corresponds to your line voltage. The use of a different input voltage other than that as indicated will cause severe damage to the microscope.

ii. Care and Maintenance

1. Do not attempt to disassemble any component including eyepieces, objectives or focusing assembly.
2. Keep the instrument clean; remove dirt and debris regularly. Accumulated dirt on metal surfaces should be cleaned with a damp cloth. More persistent dirt should be removed using a mild soap solution. **Do not use organic solvents for cleansing.**
3. The outer surface of the optics should be inspected and cleaned periodically using an air stream from an air bulb. If dirt remains on the optical surface, use a soft cloth or cotton swab dampened with a lens cleaning solution (available at camera stores). All optical lenses should be swabbed using a circular motion. A small amount of absorbent cotton wound on the end of a tapered stick makes a useful tool for cleaning recessed optical surfaces. Avoid using an excessive amount of solvents as this may cause problems with optical coatings or cemented optics or the flowing solvent may pick up grease making cleaning more difficult. Oil immersion objectives should be cleaned immediately after use by removing the oil with lens tissue or a clean, soft cloth.
4. Observe the specimen with the 4X, 10X and 40X objectives in order, then observe the specimen with the 100X objective. Apply the immersion oil on the slide cover with the 100X objective. Do not let the immersion oil to contact with the dry objectives lens (especially the 40X). Clean the dry objective lens using the lens cleaning paper if the immersion oil is on the dry objectives lens. Clean the 100X objective lens first using the lens cleaning paper after observing the specimen with the 100X objective, then clean the specimen. More persistent dirt should be removed using a little bit alcohol. **Do not use organic solvents for cleansing.**
5. Store the instrument in a cool, dry environment. Cover the microscope with the dust cover when not in use.

1. Components Illustration

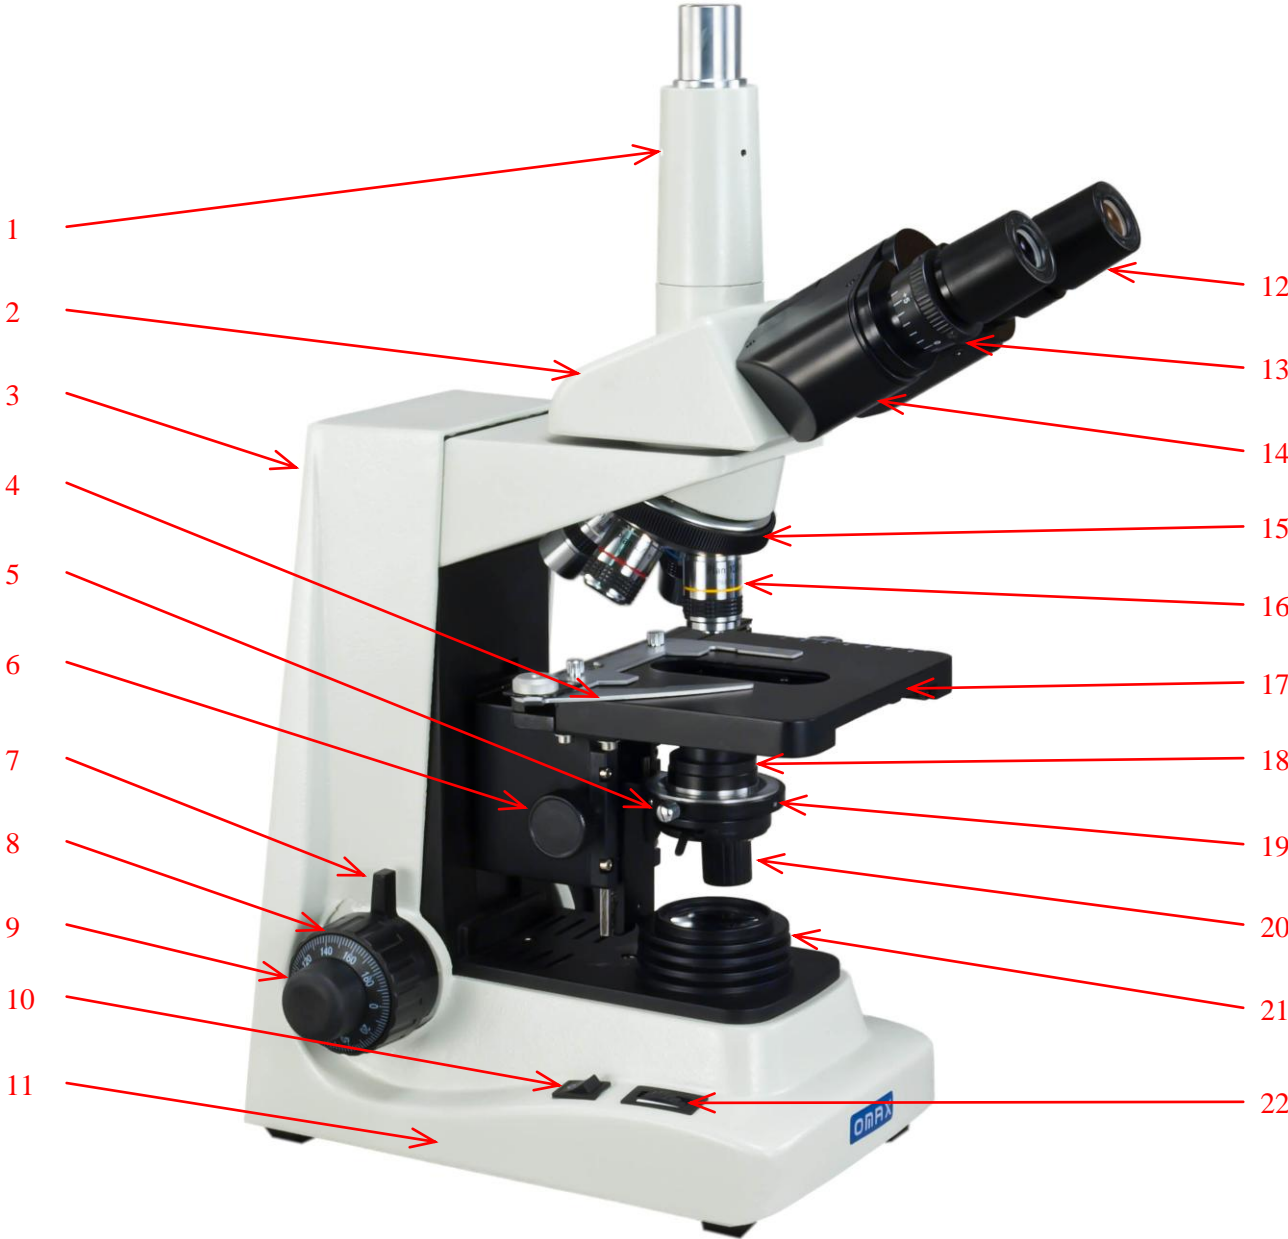

- | | | | | | |
|---|----------------------------|----|------------------------|----|---------------------------|
| 1 | Photo Tube | 9 | Fine Focus Knob | 17 | Mechanical Stage |
| 2 | Viewing Head | 10 | Power Switch | 18 | Condenser |
| 3 | Microscope Body | 11 | Microscope Base | 19 | Condenser Holder |
| 4 | Slide Holder | 12 | Eyepiece | 20 | X-Y Stage Moving Knobs |
| 5 | Condenser Lock Thumb Screw | 13 | Diopter Adjusting Ring | 21 | Light Collector |
| 6 | Condenser Focus Knob | 14 | Eyepiece Tube | 22 | Brightness Intensity Dial |
| 7 | Stage Upward Stopper | 15 | Nosepiece | | |
| 8 | Coarse Focus Knob | 16 | Objectives | | |

2. Installation

2.1 Installation of the trinocular viewing head (Fig.1)

- 1) Loosen the set screw on the top of the microscope body and remove the plastic cover.
- 2) Remove the cap on the dovetail of the trinocular viewing head.
- 3) Seat the dovetail of trinocular viewing head into the socket on the top of microscope body completely and tighten the set screw.



Fig. 1

Caution:

Do not release the viewing head from your hand grip until you are sure the viewing head is installed securely.

2.2 Installation of the photo tube

- 1) Remove the cap on the top of the viewing head.
- 2) Thread the photo tube into the top of the viewing head.

2.3 Installation of the eyepieces

- 1) Remove the protective caps from the eyepiece tubes.
- 2) Insert the eyepieces into the eyepiece tubes.

2.4 Installation of the objectives

- 1) Adjust the coarse focus knob until the mechanical stage is at its lowest position.
- 2) Turn the caps counter-clockwise to remove them from the nosepiece.
- 3) Take the objectives out from the plastic cases and turn each one clockwise into the holes on the nosepiece. Install the 4X objective into the nosepiece first. Then in a counter-clockwise direction, rotate the nosepiece and install each succeeding higher magnification objective as shown in Fig. 2.

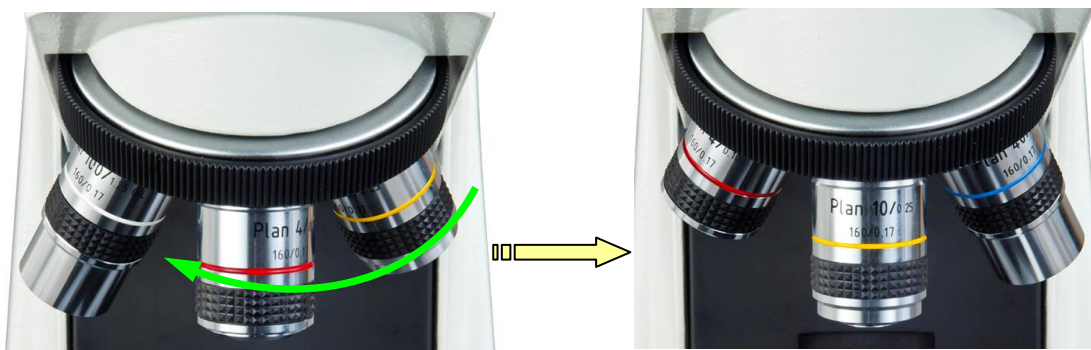


Fig.2

Note:

- Inspect the objectives frequently for dirt or oil; clean if necessary.
- Use the 10X objective to initially focus the image of your specimen.
- When changing the objective magnification, rotate the objective nosepiece until you hear a “click” sound or have a clear “in position” feeling. This ensures the objective is centered in the optical light path.

2.5 Installation of the glass color filter

- 1) Swing out the filter holder under the condenser.
- 2) Insert the filter into the holder as shown in **Fig. 3**, swing the holder in.

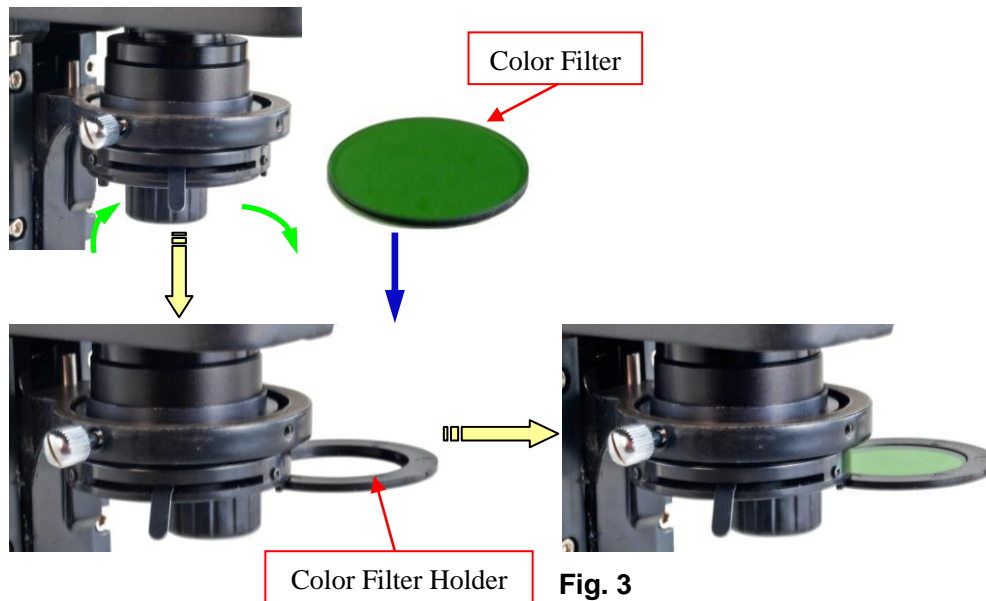


Fig. 3

2.6 Installing (or changing) the halogen bulb

- 1) Turn the power off and disconnect the power cord.
- 2) Allow some time to cool down the lamp and light housing.
- 3) Take the eyepieces off and check if the view head is securely locked by the set screw. Put the microscope down on its back gently.
- 4) Open the cover on the bottom of the base by pull the knob. Take out the dead bulb and insert the new bulb. Be sure the pins on the bulb are completely inserted into the lamp socket. See **Fig. 4**
- 5) Close the cover.

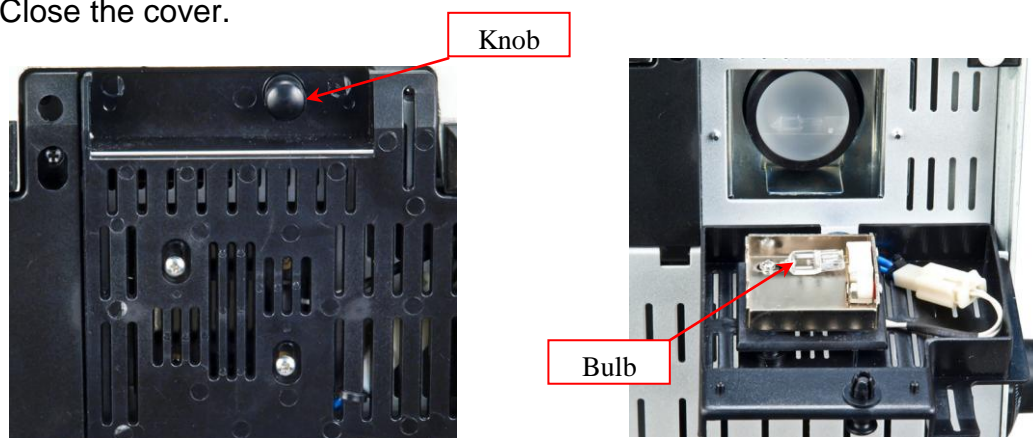


Fig. 4

Caution:

Don't touch the Halogen bulb with your bare fingers. The fingerprints left on the bulb will shorten the bulb's life.

2.7 Replacing the fuse of bottom light power supply

- 1) Turn off the power and disconnect the power cord.
- 2) Loosen the 5 screws on the back board and open the board.
- 3) Find the fuses on the board inside and take it (them) out. See **Fig. 5**.
- 4) Put in the new fuse(s) and put the board back its place.
- 5) Tighten the 5 screws.

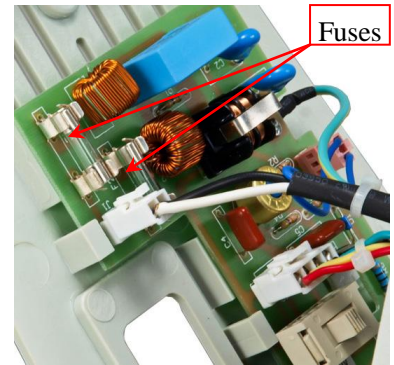


Fig. 5

2.8 Installation of the camera (optional, may not included in your package)

- 1) Take off the plastic cover from the photo tube.
- 2) Insert the camera into the photo tube, and then connect the camera to a computer via USB2.0 cable. See **Fig. 6**.
- 3) The manual for the camera is on a CD (or mini CD). Refer to the manual to install the driver and software on to the computer.
- 4) The camera is optional and may have different color and shape from the one in the figure, depending on the model purchased.

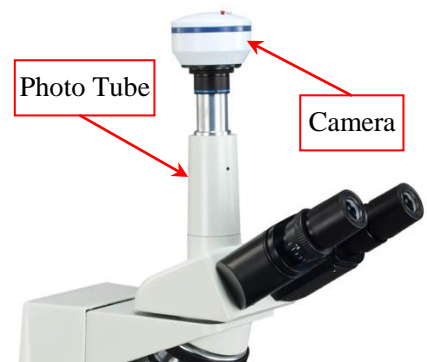


Fig. 6

2.9 Installation of darkfield condensers (optional, may not included in your package)

Please see section 7 (*Darkfield Condenser Installation and Operation Instructions*)

2.10 Installation of phase contrast kit (optional, may not included in your package)

Please see section 8 (*Phase Contrast Kit Installation and Operation Instruction*)

3. Operation

3.1 Adjusting illumination

- 1) Plug the power cord into the power socket on the microscope and connect it to the power outlet.
- 2) Turn on the power switch.
- 3) Rotate the brightness intensity dial to increase or decrease the brightness.

Caution:

A diffusion filter is attached beneath the condenser to get uniform light and protect your eyes from strong light when a low power objective applied. The diffusion filter can be swung out to make the view field brighter when observing with a high power objective, such as 100X objective.

3.2 Placing specimen

- 1) Place the slide on the mechanical stage.
- 2) Use the slide holder to gently secure the slide.
- 3) Turn the X-Y stage moving knobs to position the specimen in the center of viewing head.

Caution:

Be sure not to allow an objective to touch a specimen slide when changing objectives.

3.3 Focusing

- 1) With the 10X objective in position, raise the mechanical stage using the coarse focus knob until the specimen is close to the objective.
- 2) Turn the coarse focus knob until the specimen is in focus.
- 3) Use the fine focus knob to obtain a sharp image.
- 4) To get a good focused image, you may need to combine the focus knob adjustment and interpupillary distance adjustment, along with eyepiece diopter adjustment stated in **3.6** and **3.7**.
- 5) You may now switch to another magnification objective.

Tips:

To prevent your specimen slide from making contact with an objective, raise the stage to its highest position without contacting the 100X objective, then tighten the stage upper stopper (**Fig. 7**). Give the stage a tiny extra moving space to ensure the objective can be focused every time.

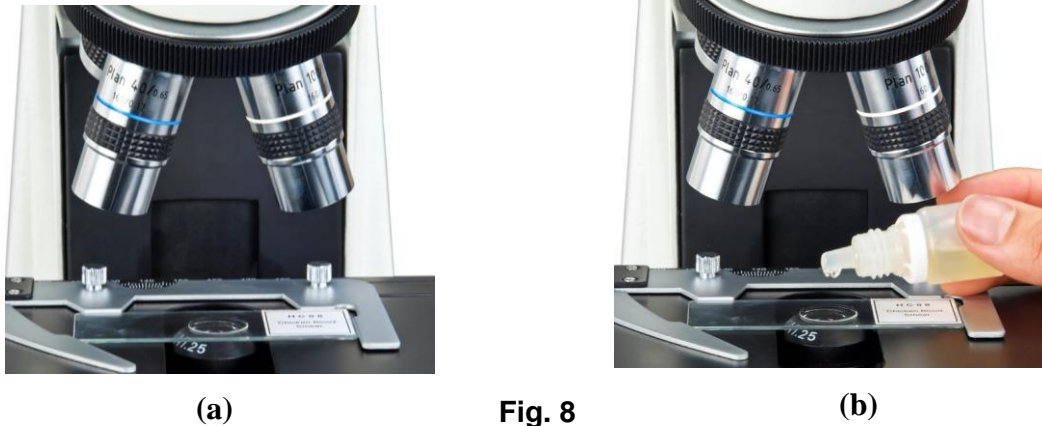


Fig. 7

3.4 Applying the immersion oil

- 1) Rotate the objective nosepiece to seat the observing position between the 40X and 100X objectives as shown in **Fig. 8 (a)**.
- 2) Place a drop of immersion oil on the slide cover as shown in **Fig. 8 (b)**.
- 3) Rotate the objective nosepiece to seat the 100X objective to the observing position until you hear a “click” sound.
- 4) After observing the specimen, use the lens cleaning paper to clean the 100X objective lens gently and the specimen in time.

- 5) If it is hard to clean, you need a little bit alcohol to clean the 100X objective lens and the specimen.



Caution (important):

- When you use the 100X objective to observe the specimen, you have to finish observing the specimen with the 4X, 10X, 40X objectives.
- When you use the 100X objective to observe the specimen, you have to apply the immersion oil on the top of the slide cover.
- When you apply the immersion oil with the 100X objective, do not let the immersion oil to contact with the dry objective lenses (especially the 40x). If the immersion oil is on the dry objectives lens, please use the lens cleaning paper to clean the objectives lens in time. The oil will damage the dry objective lenses.
- After observing the specimen with the 100X objective, clean the 100X objective lens first.

3.5 Adjusting condenser

- 1) Turn the condenser focus knob to raise or lower the condenser.
- 2) The condenser is raised when using high magnification objectives and lowered when using low magnification objectives.

Note:

- The centering of the condenser and the light axis of the objective are factory adjusted. Do not attempt re-adjustment.
- The highest position of the condenser has been factory adjusted. Do not attempt re-adjustment.

3.6 Adjusting interpupillary distance

While observing with both eyes, hold the left and right eye tubes, swing inwards and outwards. The interpupillary distance is correct when the left and right fields of view converge completely into one image.

3.7 Adjusting eyepiece diopter

- 1) Using the 10X objective and your right eye only, observe your specimen through the eyepiece and bring it into focus by adjusting the focus knobs.
- 2) Then observe the specimen with your left eye only through the left eyepiece. If the specimen is not in focus, rotate the diopter ring until a sharp image is obtained.

3.8 Adjusting Iris diaphragm

Swing the iris diaphragm lever (**Fig. 9**) left or right to adjust the aperture size.

Note:

The iris diaphragm is designed to adjust the aperture size, not to adjust the brightness although the brightness will be changed when it's adjusted. When aperture is adjusted to smaller size, the contrast will be increased and the depth of field will be increased as well. Turn up the intensity of the light if the image is too dim.



Fig.9

3.9 Adjusting focus tension

The focus tension has been pre-set at the factory. If the mechanical stage drops by itself, rotate the focus tension ring (**Fig. 10**) situated between the coarse focus knob and microscope body on the right side until the tension is in maintained.



Fig.10

3.10 Camera (optional, may not included in your package)

- 1) Bring the microscope into focus by following the procedures in **3.3**.
- 2) Install the camera by following the procedures in **2.8**.
- 3) Open image observing software to examine (more details see camera's manual).
- 4) If the image is not clear, loosen the set screws (See **Fig. 11**) on the photo tube, turn the upper half part to lower down or raise up the camera mounted on the top, till the image is clear.
- 5) You also can capture images or record live videos through the software, depending on the functions provided by the software.

Note:

Please refer to the manuals in the camera's CD for the details of installation and operation of the camera.



Fig.11

3.11 Darkfield condensers observation (optional, may not included in your package)

Please see section 7 (*Darkfield Condenser Installation and Operation Instructions*)

3.12 Phase contrast kit observation (optional, may not included in your package)

Please see section 8 (*Phase Contrast Kit Installation and Operation Instruction*)

4. Specifications







General

| | |
|--|---|
| Model | M834PLAN series |
| Total Magnification | 40X, 64X, 100X, 160X, 400X, 640X, 1000X, 1600X |
| Viewing Head | Trinocular, Siedentopf, inclined 30°, swiveling 360° Swing interpupillary adjustment, 2-3/16" ~ 2-15/16" (55 ~ 75mm) Adjustable diopter on left eyepiece tube |
| Photo Tube | Height adjustable |
| Eyepieces | 1 pair of WF10X/18 1 pair of P16X |
| Objective Tube Length | 160mm |
| Nosepiece | Reversed revolving quadruple |
| Objectives | PLAN 4X, 10X, 40X (spring), 100X (spring, oil) |
| Condenser | Abbe, NA=1.25, w/ iris diaphragm and filter holder Rack and pinion adjustment |
| Focus Mechanism | Coaxial coarse and fine focusing knobs on both sides w/ stage upward stopper Minimum fine focusing adjustment at 0.002mm, range 30mm |
| Mechanical Stage | Large double layer mechanical stage Dimension: 5-1/2" x 4-1/4" (140mmx110mm) Movement range: 3" x 2" (78mm X 52mm) |
| Cameras (<i>optional</i>) | Refer to the cameras specifications |
| Darkfield Condensers (<i>optional</i>) | Refer to the darkfield condensers specifications |
| Phase Contrast Kit (<i>optional</i>) | Refer to the phase contrast kit specification |
| Carrying Case (<i>optional</i>) | Net weight: 9 lbs 4.5 oz (4.25 kg) Size: 17-1/2" x 11-1/4" x 14-1/8" (44.5cm x 28cm x 36cm) |
| Illumination | Transmitted: 6V/20W, halogen, variable intensity |
| Power Supply | AC 110V-115V, 50/60HZ (US and Canada plug) (220V version available, contact seller) |
| Dimension | 14-1/8" x 9-1/8" x 19" (36cm x 23cm x 48cm) |
| Net weight | 20 lbs (9 kg) |



5. Optional Parts

The optional parts may be included in some models or sold separately.)





1) Cameras

| | Model | Resolution | Operating System | Software |
|---|--------|---------------------|-------------------------------------|----------|
|  | A1502 | 640 x 480 (0.3MP) | MS Windows (32/64-bit) Mac OS | Included |
|  | A1510 | 1280 x 1024 (1.3MP) | | |
|  | A1520C | 1600 x 1200 (2.0MP) | | |
|  | A1530X | 2048 x 1536 (3.0MP) | | |
|  | A1550X | 2592 x 1944 (5.0MP) | | |
|  | A1590 | 3488 x 2616 (9.0MP) | MS Windows (32/64-bit) | |

2) Darkfield Condensers

| | Model | Darkfield Condenser | Numerical Aperture | Objective | Mounting Size(diameter) |
|---|----------|---------------------|--------------------|--|-------------------------|
|  | A191 | Dry | 0.7-0.9 | - | 37mm |
|  | A191BOIL | Oil | 1.36-1.25 | Plan 100X/1.25 oil-0.5 160/0.17(Spring), w/ iris diaphragm | 37mm |

3) Phase Contrast Kits

| | Model | Phase Contrast Objective | Condenser | Annular Ring Plates | Centering Telescope |
|---|--------|--|-----------|--|---------------------|
|  | A1PHB1 | Plan achromatic 10X with built-in phase plate Plan achromatic 20X with built-in phase plate Plan achromatic 40X with built-in phase plate, spring Plan achromatic 100X with built-in phase plate, spring, oil | NA 1.25 | five positions: 10 for 10X phase contrast objective 20 for 20X phase contrast objective 40 for 40X phase contrast objective 100 for 100X phase contrast objective B for bright field observation, with iris diaphragm | focusing adjustable |
|  | A1PHB3 | Achromatic 10X with built-in phase plate Achromatic 20X with built-in phase plate Achromatic 40X with built-in phase plate, spring Achromatic 100X with built-in phase plate, spring, oil | | five positions: 10 for 10X phase contrast objective 20 for 20X phase contrast objective 40 for 40X phase contrast objective 100 for 100X phase contrast objective B for bright field observation, with iris diaphragm | |
|  | A1PHC1 | Plan achromatic 10X with phase plate Plan achromatic 40X with phase plate | | three positions: 10 for 10X phase contrast objective 40 for 40X phase contrast objective middle position for brightfield observation | |
|  | A1PHD | Achromatic 10X with built-in phase plate Achromatic 40X with built-in phase plate, spring Achromatic 100X with built-in phase plate, spring, oil | | 10 for 10X phase contrast objective 40 for 40X phase contrast objective 100 for 100x phase contrast objective | |

6. Troubleshooting Guide

GENERAL PROBLEMS

| Problem | Cause | Solution |
|---|--|--|
| Lamp does not light when switched on | No electrical power | Check power cord connection |
| | Lamp bulb burnt out | Replace bulb |
| | Fuse blown out | Replace fuse |
| Darkness at the periphery or uneven brightness in the field of view | Revolving nosepiece not in click stop position | Revolve the nosepiece to click-stop position by swinging the objective correctly into the optical path |
| | The light source of the bulb is not at the center | Adjust the position of the bulb |
| Dirt or dust on the view | Dirt or dust on the eyepiece, condenser, objective or collector lens or specimen | Clean the lens with a lens cleaning paper |
| Poor image quality or not able to get focused image | No slide cover attached to the slide | Attach a 0.17mm slide cover |
| | Slide cover is too thick or thin | Use a slide cover of the appropriate thickness (0.17mm) |
| | Slide may be upside down (specimen at the bottom) | Turn slide over so the cover-glass faces up |
| | Immersion oil is on a dry objective (especially the 40X) | Check the objectives, clean if necessary |
| | No immersion oil used with 100X objective | Use immersion oil |
| | Air bubbles in immersion oil | Remove bubbles |
| | Condenser aperture is closed or open too much | Open or close properly |
| | Condenser is positioned too low | Position the condenser upward |
| | Specimen rises from stage surface | Secure the specimen in the slide holder |
| | Blue filter not used | Use daylight blue filter |
| | Lamp intensity is too high or low | Adjust the light intensity by rotating the intensity control dial |
| Slippage of focus when using the coarse focusing knob Fine focus is ineffective | Tension adjustment is set too low | Increase the tension on the focusing knobs |
| | Tension adjustment is set too high | Loosen the tension on the focusing knobs |

DARKFIELD PROBLEMS

| Problem | Cause | Solution |
|---|--|---|
| It's totally dark in the viewing field | The light is not on | Turn on the light |
| | <i>(A191BOIL only)</i> There is no oil in between the condenser top lens and slide | Place a drop of oil on the top lens of condenser and let it contact the underside of slide |
| | <i>(A191BOIL only)</i> The built-in iris diaphragm of 100X objective is not in proper position | Adjust the iris diaphragm ring on the objective |
| | The condenser is not in the right position | Lower or raise the condenser slightly to the position that the specimen is the brightest. <i>(A191BOIL only)</i> Make sure the oil contact the bottom of the slide and the top of the condenser during the adjustment. |
| The illumination is insufficient or too bright | The intensity of lamp is too low | Adjust the intensity dial to increase the brightness |
| | The condenser is not in the right position | Lower or raise the condenser slightly to the position that the specimen is the brightest. <i>(A191BOIL only)</i> Make sure the oil contact the bottom of the slide and the top of the condenser during the adjustment. |
| | The condenser is not centered properly | Adjust the translational centering screws to center the condenser |
| | <i>(A191BOIL only)</i> The built-in iris diaphragm of 100X objective is not in proper position | Turn the iris diaphragm ring on the objective |
| Image of the specimen is not clear and lacking in sufficient contrast | The specimen is not suitable for darkfield observation | Change to brightfield or phase contrast |
| | <i>(A191BOIL only)</i> The built-in iris diaphragm of 100X objective is not in proper position | Turn the iris diaphragm ring on the objective |
| | The condenser is not in the right position | Lower or raise the condenser slightly to the position that the specimen is the brightest. <i>(A191BOIL only)</i> Make sure the oil contact the bottom of the slide and the top of the condenser during the adjustment. |

7. Darkfield Condenser Installation and Operation

Instructions

7.1 Dry darkfield condenser of A191

- 1) Mounting the dry darkfield condenser
 - Loosen the condenser lock thumb screw on the condenser holder and remove the brightfield condenser.
 - Install the dry darkfield condenser and tighten the condenser lock thumb screw on the condenser holder (see **Fig. 12**).
- 2) Centering the dry darkfield condenser
 - Turn the 4X objective to the light path.
 - Turn the condenser focus knob to lower the condenser till a dark spot showed in the viewing field as shown in **Fig. 13 (a)**.
 - Turn the condenser translational centering screws to move the dark spot to the center as shown in **Fig. 13 (b)**.
- 3) Place the slide on the stage.
- 4) Raise the condenser all the way to the top and lower it a little bit.
- 5) Following the procedures in this manual to focus and observe.
- 6) Move the condenser up or down slightly to get the best darkfield viewing.

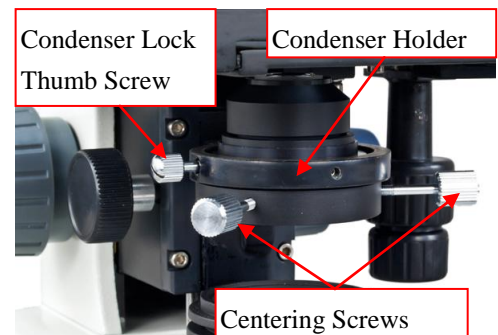


Fig.12

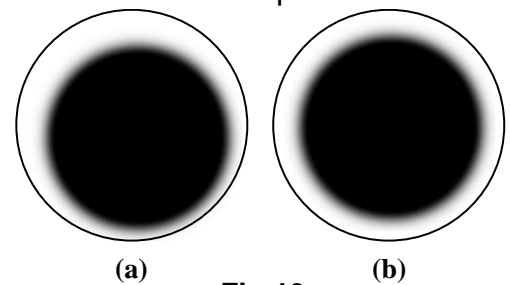


Fig.13

Note:

- The dry darkfield condenser is used with the dry objectives only.
- The dry darkfield condenser works with the 4X, 10X, 40X objectives.
- The dry darkfield condenser won't work with the 100X oil immersion objective.

7.2 Oil darkfield condenser of A191BOIL

- 1) Mounting the oil darkfield condensers
 - Loosen the condenser lock thumb screw on the condenser holder and remove the brightfield condenser.
 - Install the oil darkfield condensers and tighten the condenser lock thumb screw on the condenser holder (see **Fig. 14**).
- 2) Centering the oil darkfield condensers
 - Turn the 40X objective to the light path.
 - Turn the condenser focus knob to slowly lower and raise the condenser till a dark spot showed in the viewing field as shown in **Fig. 15 (a)**.
 - Turn the condenser translational centering screws to move the dark spot to the center as shown in **Fig. 15 (b)**.

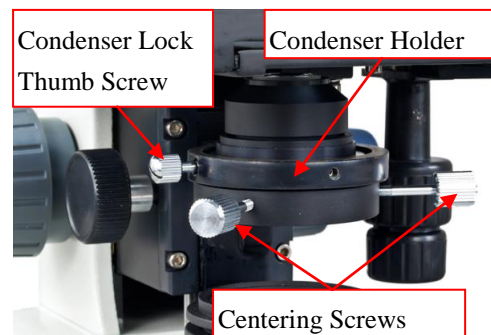


Fig.14

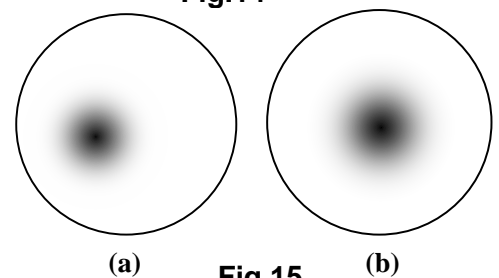


Fig.15

- 3) Raise the condenser till the top lens is close to the opening of stage. Place a drop of immersion oil on the top of the lens of the condenser.
- 4) Place the slide on the stage. Raise the condenser and let the oil drop contact the bottom of the slide. If air bubbles exist in the oil, clean the oil from the condenser lens and bottom of slide with a camera cleaning paper and repeat the procedures.
- 5) Follow the procedures in this manual to bring the sample on slide in focus and observe.
- 6) When using the 100X oil darkfield objective, you will need to drop the immersion oil and adjust the iris ring (**Fig. 16**) to get proper brightness and contrast of view field.



Fig.16

Note:

- The condenser won't work well if no oil drop applied on the condenser.

8. Phase Contrast Kit Installation and Operation Instructions

8.1 Phase contrast kits of A1PHB1 or A1PHB3:

- 1) Mounting the phase contrast objectives
 - a. Take off all the objectives from the nosepiece.
 - b. Install the phase contrast objectives onto the nosepiece following the steps in 2.4.
- 2) Mounting the phase contrast condenser/annular ring disk
 - a. Rotate the nosepiece and set the 4X objective in position.
 - b. Turn the coarse focus knob to raise the mechanical stage to the highest position without contacting the 4X objective.
 - c. Turn the condenser control knob to raise the condenser to the highest position.
 - d. Loosen the condenser lock thumb screw, pull down the condenser and take it off.
 - e. Insert the condenser/annular ring disk into the condenser holder, and tighten the thumb screw.
 - f. Re-adjust the condenser height to its normal position.
 - g. Re-adjust the mechanical stage height to its normal position.

Note:

- When raising the mechanical stage, do not make contact with the objective.
- 3) Turn the desired objective into light path.
 - 4) Turn the annular ring disk to put the corresponding ring into light path, i.e. if you are using the 20X phase contrast objective, you should turn the disk at 20 as shown in **Fig. 17**.



Fig.17

- 5) Centering the annular ring.
 - a. Remove one eyepiece from the microscope eyepiece tube and insert the centering telescope as shown in **Fig. 18**.
 - b. Observe from the telescope. The bright ring and dark ring should be coincided with each other as shown in **Fig. 19 (d)**.
 - c. If the ring images are not clear, turn the top of telescope until both ring images are in focus.
 - d. If the bright ring is still obscure as in **Fig. 19 (b)**, adjust the condenser focus knob.
 - e. If the two ring images are not coincided as shown in **Fig. 19 (c)**, hold the ring plate from the bottom of the annular ring disk and adjust its position until two ring images are coincided.
 - f. Remove the centering telescope and replace it with the eyepiece.
 - g. Put the specimen on the stage and adjust the illumination, focusing, etc following the instructions in this manual.



Fig.18

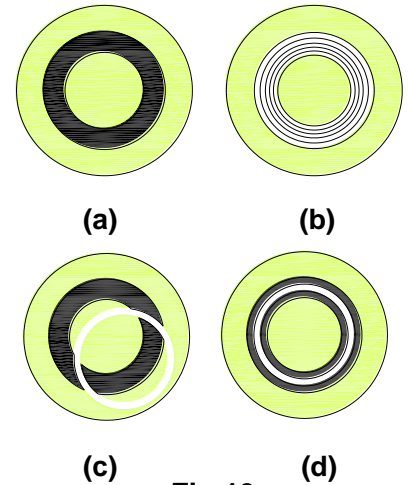


Fig.19

Note:

- The phase contrast condenser will be working as a conventional Abbe condenser if the annular ring disk being put at B position.

8.2 Phase contrast kit of A1PHC1:

- 1) Mounting the phase contrast kit
 - a. Replace the bright field objective(s) on nosepiece with the phase contrast objective(s).
 - b. Rotate the nosepiece and set the 4X objective in position.
 - c. Turn the coarse focus knob to raise the mechanical stage to the highest position without contacting the 4X objective.
 - d. Turn the condenser control knob to raise the condenser to the highest position.
 - e. Loosen the condenser lock thumb screw (**Fig. 20**), pull down the condenser and take it off.
 - f. Insert the condenser/annular ring disk into the condenser holder, and tighten the thumb screw (**Fig. 20**).
 - g. Re-adjust the condenser height to its normal position.
 - h. Re-adjust the mechanical stage height to its normal position.

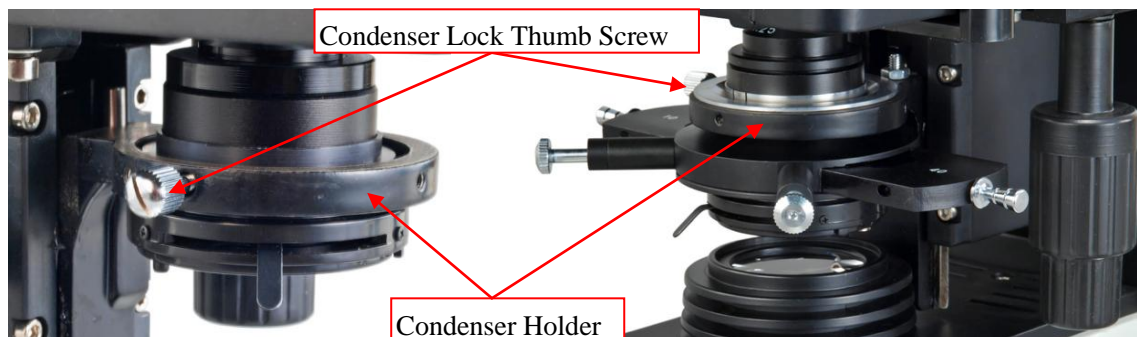


Fig.20

Note: there are 2 phase contrast objectives: 10X and 40X, and there are 2 condenser annular rings on the annular ring switch: 10X and 40X. The corresponding objective and annular ring must work together, i.e. 10X phase contrast objective must work with 10X condenser annular ring, and so on.

2) Centering the condenser ring plate

- a. Connect the power cord to the microscope and insert the plug into a power outlet.
- b. Turn the desired phase contrast objective into light path. Slide the annular ring switch to the required annular ring corresponding to the phase contrast objective in the light path.
- c. Remove one eyepiece from the microscope eyepiece tube and insert the centering telescope.
- d. Observe from the telescope. The bright ring and dark ring should be coincided with each other as shown in **Fig. 21 (d)**.
- e. If the ring images are not clear, turn the top of telescope until both ring images are in focus.
- f. If the bright ring is still obscure as in **Fig. 21 (b)**, adjust the condenser focusing knob.
- g. If the two ring images are not coincided as shown in **Fig. 21 (c)**, adjust the two centering screws on the phase contrast condenser.
- h. Remove the centering telescope and replace the eyepiece.

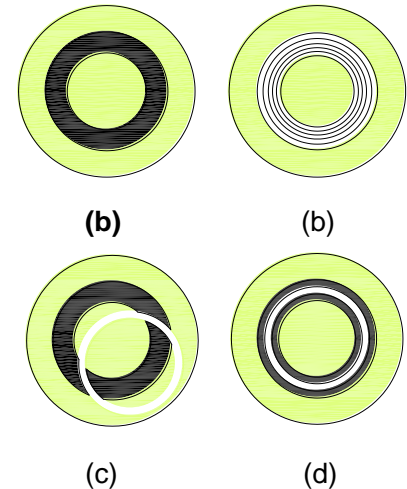


Fig. 21

8.3 Phase contrast kit of A1PHD:

- 1) Mounting the phase contrast kit
 - a. Replace the bright field objective(s) on nosepiece with the phase contrast objective(s)
 - b. Thread the condenser ring plate onto the condenser as shown in **Fig.22**.
 - c. Loosen the condenser lock thumb screw as shown in **Fig. 23**; take off the original condenser from the holder.
 - d. Insert the phase contrast condenser into the condenser holder as shown in **Fig. 23**; tighten the condenser lock thumb screw.



Fig.22

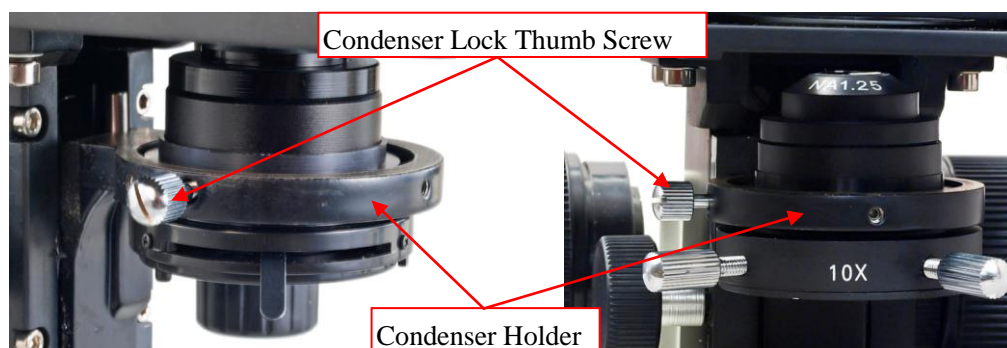


Fig. 23

Note: there are 3 phase contrast objectives: 10X, 40X and 100X, and there are 3 condenser ring plates: 10X, 40X and 100X. The corresponding objective and ring plate must work together, i.e. **10X** phase contrast objective must work with **10X** condenser ring plate, and so on.

2) Centering the condenser ring plate

a. Connect the power cord to the microscope and insert the plug into a power outlet.
b. Turn the desired phase contrast objective into light path.

c. Choose the ring plate that corresponding to the phase contrast objective in light path and screw it on the condenser.

d. Replace the bright field condenser with the phase contrast condenser with ring plate on.

e. Remove one eyepiece from the microscope eyepiece tube and insert the centering telescope.

f. Turn the light of microscope on and observe from the telescope.

g. Turn the top of the telescope (**Fig.25**) until the dark ring image is in focus. If the dark ring is hard to find, put a normal white print paper on the stage and under the objective then you will see the dark ring as shown in **Fig.24 (a)**.

h. If the bright ring is still obscure as in **Fig.24 (b)**, raise or lower the condenser by adjusting the condenser focusing knob (or the microscope focusing knob if necessary) till the bright ring is in focus and the dark ring is visible.

i. If the two ring images are not coincided as shown in **Fig.24 (c)**, adjust the two centering screws on the condenser ring plate till the two rings are coincided with each other as shown in **Fig.24 (d)**.

j. Remove the centering telescope and replace it with the eyepiece.

3) Performing the phase contrast observation

After you center the ring plate, you can perform the phase contrast observation the same way as a normal bright field microscope.

Note: when change to another phase contrast objective and corresponding condenser ring plate, the focusing and centering of bright ring and dark ring should be repeated following the procedures from **2)-b to 2)-h**.

Tips:

- Make the illumination as bright as possible.
- The thinner the specimen, the better the image.

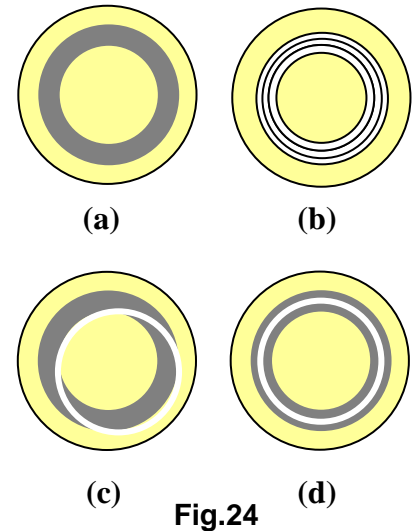


Fig.24



Fig.25