AMENDMENT OF SOLICITATION/MODIFICATION OF CONTRACT

BPA NO.	1. CONTRACT ID CODE	PAGE OF PAGES

2. AMENDMENT/MODIFICATION NUMBER	3. EFFECTIVE DATE	4. REQUISITION/PURCHASE REQ. NUMBER	5. PROJECT NUMBER (if applicable)
0001		595-27-1-082-0004	None

6. ISSUED BY	CODE	7. ADMINISTERED BY (If other than Item 6)	CODE
Department of Veterans Affairs Network Contracting Office 4 H.J. Heinz VA Medical Center 1010 Delafield Road Pittsburgh PA 15215	00244	Department of Veterans Affairs Network Contracting Office 4 H.J. Heinz VA Medical Center 1010 Delafield Road Pittsburgh PA 15215	00244

8. NAME AND ADDRESS OF CONTRACTOR (Number, street, county, State and ZIP Code)	(X)	9A. AMENDMENT OF SOLICITATION NUMBER
To all Offerors/Bidders		36C24427Q0039
	X	9B. DATED (SEE ITEM 11)
		10A. MODIFICATION OF CONTRACT/ORDER NUMBER
		10B. DATED (SEE ITEM 13)
CODE / FACILITY CODE		

11. THIS ITEM ONLY APPLIES TO AMENDMENTS OF SOLICITATIONS

[X] The above numbered solicitation is amended as set forth in Item 14. The hour and date specified for receipt of Offers [X] is extended, [ ] is not extended.

Offers must acknowledge receipt of this amendment prior to the hour and date specified in the solicitation or as amended, by one of the following methods:

(a) By completing Items 8 and 15, and returning _____ copies of the amendment; (b) By acknowledging receipt of this amendment on each copy of the offer submitted; or (c) By separate letter or electronic communication which includes a reference to the solicitation and amendment numbers. FAILURE OF YOUR ACKNOWLEDGMENT TO BE RECEIVED AT THE PLACE DESIGNATED FOR THE RECEIPT OF OFFERS PRIOR TO THE HOUR AND DATE SPECIFIED MAY RESULT IN REJECTION OF YOUR OFFER. If by virtue of this amendment you desire to change an offer already submitted, such change may be made by letter or electronic communication, provided each letter or electronic communication makes reference to the solicitation and this amendment, and is received prior to the opening hour and date specified. ** HOUR & DATE for Receipt of Offers is EXTENDED to: 11-24-2026 4:30PM EST

12. ACCOUNTING AND APPROPRIATION DATA (If required)

13. THIS ITEM APPLIES ONLY TO MODIFICATIONS OF CONTRACTS/ORDERS, IT MODIFIES THE CONTRACT/ORDER NO. AS DESCRIBED IN ITEM 14.

CHECK ONE	
[ ]	A. THIS CHANGE ORDER IS ISSUED PURSUANT TO: (Specify authority) THE CHANGES SET FORTH IN ITEM 14 ARE MADE IN THE CONTRACT ORDER NO. IN ITEM 10A.
[ ]	B. THE ABOVE NUMBERED CONTRACT/ORDER IS MODIFIED TO REFLECT THE ADMINISTRATIVE CHANGES (such as changes in paying office, appropriation date, etc.) SET FORTH IN ITEM 14, PURSUANT TO THE AUTHORITY OF FAR 43.103(b).
[ ]	C. THIS SUPPLEMENTAL AGREEMENT IS ENTERED INTO PURSUANT TO AUTHORITY OF:
[ ]	D. OTHER (Specify type of modification and authority)

E. IMPORTANT: Contractor [X] is not, [ ] is required to sign this document and return _____ copies to the issuing office.

14. DESCRIPTION OF AMENDMENT/MODIFICATION (Organized by UCF section headings, including solicitation/contract subject matter where feasible.)

The purpose of this amendment is for the following:
1. To submit all the questions and the answeres
2. To change 52.219-6 - Total Small Business Set-Aside to 52.219-30 - Total Women Owned Business.
3. The last days for questions is 11-13-2026.
4. To extend the due date for proposal to 11-24-2026 by 4:30PM EST.

Except as provided herein, all terms and conditions of the document referenced in Item 9A or 10A, as heretofore changed, remains unchanged and in full force and effect.

15A. NAME AND TITLE OF SIGNER (Type or print)		16A. NAME AND TITLE OF CONTRACTING OFFICER (Type or print)	
		Amanda Saunders Contract Specialist	
15B. CONTRACTOR/OFFEROR (Signature of person authorized to sign)	15C. DATE SIGNED	16B. UNITED STATES OF AMERICA (Signature of Contracting Officer)	16C. DATE SIGNED

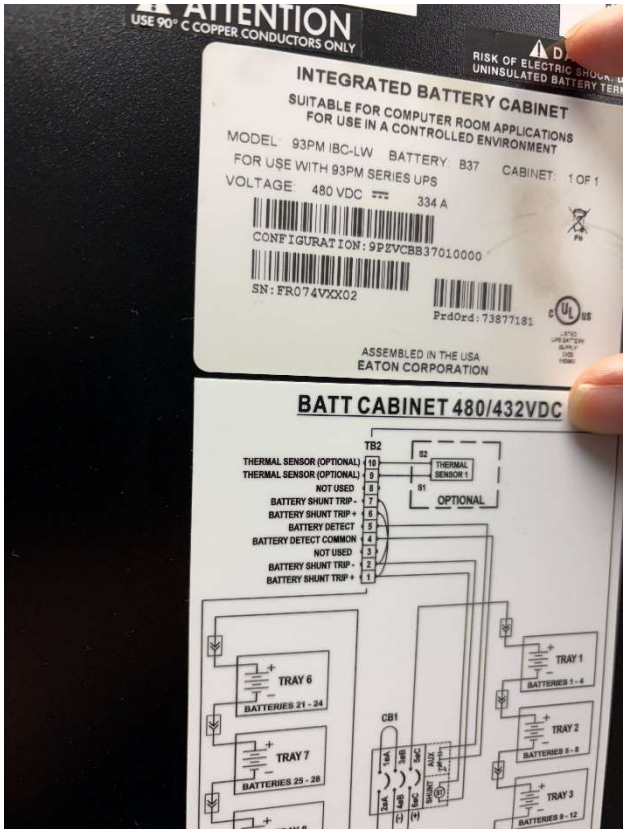
Extension

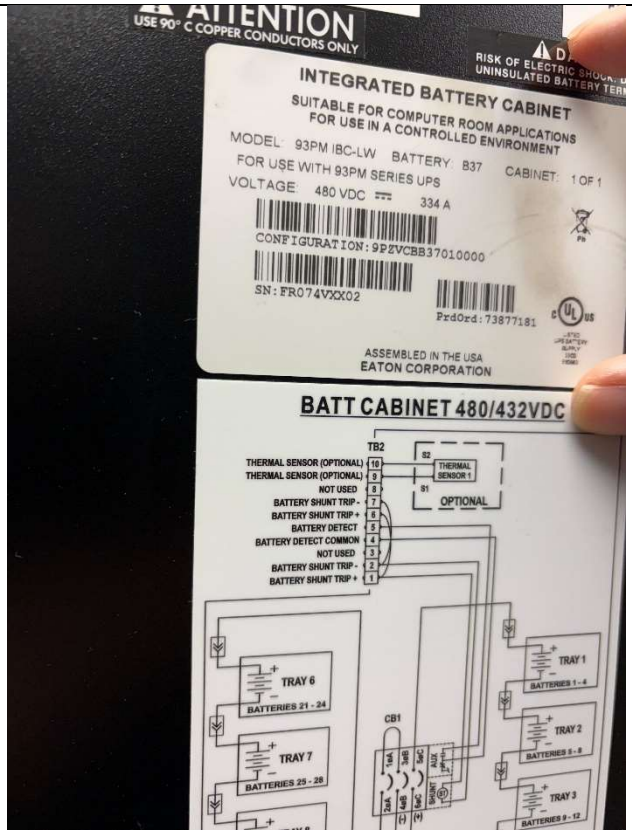
FAR Number	Title	Date
52.219-30	NOTICE OF SET-ASIDE FOR, OR SOLE-SOURCE AWARD TO, WOMEN-OWNED SMALL BUSINESS CONCERNS ELIGIBLE UNDER THE WOMEN-OWNED SMALL BUSINESS PROGRAM (DEVIATION)	NOV 2025

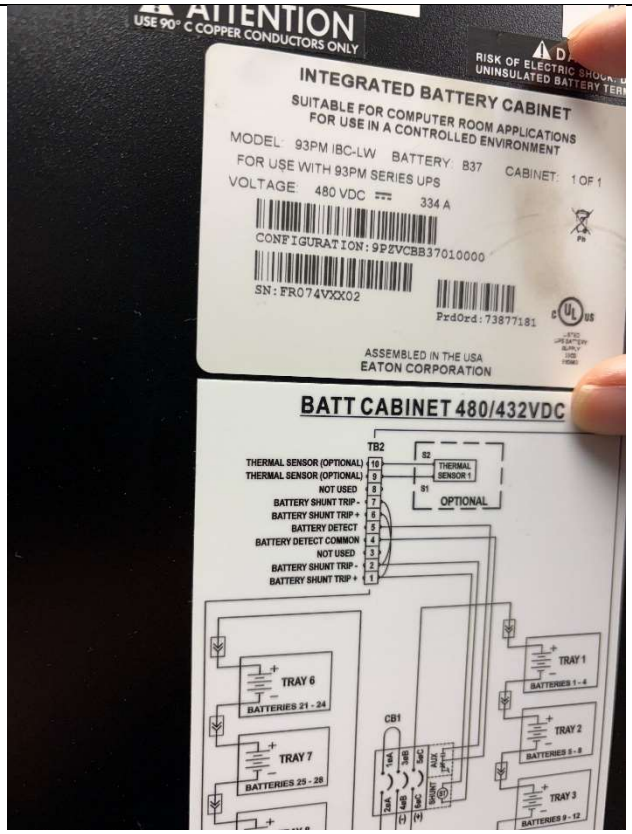
Uninterrupted Power Supply (UPS) Batteries/Solicitation #36C24427Q0039 | Lebanon VA Medical Center

Question and Answers

Number	Vendor Question	Government Response
1	Testing scope. Statement of Need paragraph VI requires a full functional test of the UPS system to verify proper operation, voltage outputs, and battery backup capabilities. Please clarify which of the following the Government expects: a) A functional test: close the battery breaker, confirm no alarms, record float voltage and individual battery readings, and verify transfer to battery and back; or b) The above plus a load bank discharge test verifying battery runtime, with a written report. A load bank test adds significant cost, so this answer will let every offeror price the same scope.	A is required, B is not required

2	Addition to the UPS details requested below, please provide its serial number and, if available, a photo of the manufacturer's identification plate or site ID/tag label.	 

3	UPS details. The Statement of Need identifies the batteries (C&D Technologies VRLA Sealed UPS12-400MR) but not the UPS unit they serve. Could you provide the UPS manufacturer, model and kVA rating, and the number of battery strings? Our installation partner needs this to plan the functional test required under Statement of Need paragraph VI. If a site visit can be arranged before the 11-17-2026 due date, we would welcome one.	
4	Will a product made outside the US be accepted under Buy American? C+D is manufactured in Mexico	Must be Trade Agreements Act (TAA) complaint.

5	Can photos of the battery string and UPS nameplate be provided?	 We do not have a photo of the Battery string and Do not want to open the UPS to get one.
6	C&D Technologies' retired product listing identifies the specified UPS12-400MR as retired and lists UPS12-405PLP as its replacement. Please confirm whether the Government will accept this replacement model. Please also confirm whether batteries from other manufacturers that meet or exceed all specified salient characteristics and are compatible with the existing UPS system will be considered.	Retired Products page lists UPS12-400MR as a retired model with UPS12-405PLP as its replacement This replacement is acceptable.

Number	**Vendor Question**	**Government Response**
8	Is there an on-site location where the old batteries can be staged for pickup or do they need to be removed same day as job?	We prefer that the batteries be removed the same day. There is a space for these to be staged in the Biomed Workshop if the staging time is less than 5 days.
9	What is the path from delivery to Room G034 (elevator, distance.	The loading dock in Building 1 is on the same level as room G034. And there is one double door that is not locked on the way. It is about 300 ft.
10	Is any test documentation required beyond the functional test?	Provide a copy of a completed functional test check list.
11	Can batteries be delivered ahead of the install date or do they need to deliver same day as installation?	We prefer that the batteries be delivered on the day of installation. If needed and if internal delivery is provided, the batteries can be stored in the Biomedical Engineering department in Building 1 3rd floor for up to 5 days.

End of Document