Star Care

Fișă tehnică

Mască FFP2 Star Care

1 Informații tehnice

- **Denumirea produsului:** Mască de filtrare
- **Clasificare** FFP2 - NR (de unică folosință)
- **Model:** MSH
- **PFE** > 94 % [>98 % pentru aerosoli de clorură de sodiu (NaCl)]
- **Dimensiuni:** 157 mm x 107 mm
- **Standard respectat:** EN 149:2001 + A1:2009
- **Compoziție:** 66,7 % țesătură nețesută, 33,3% țesătură suflată topită
- **Notificare alergii:** Textile nețesute
- **Valabilitate:** Doi ani în condițiile de depozitare specificate

2 Imagini reale ale produsului

Star Care
NR
No reutilizable
Non-reusable
1 UD / 1 PC
FFP2
Mascarilla filtrante - NR
Filtering half mask
Ajuste perfecto
Perfect fit
Incluye salvaorejas
Ear saver included
Bolsa zip porta mascarillas
Zip bag for masks
Información técnica
Technical information
22092020
HE23-0001
CE 2163

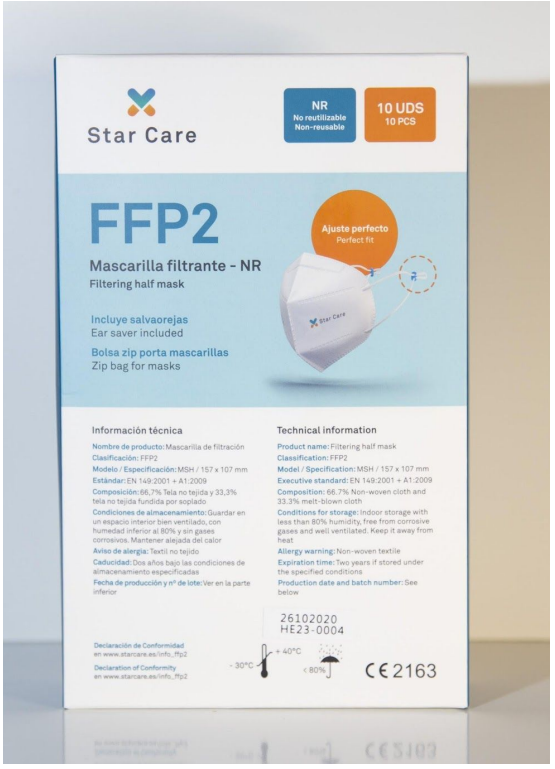
Star Care
NR
No reutilizable
Non-reusable
10 UDS
10 PCS
FFP2
Mascarilla filtrante - NR
Filtering half mask
Ajuste perfecto
Perfect fit
Incluye salvaorejas
Ear saver included
Bolsa zip porta mascarillas
Zip bag for masks
Información técnica
Technical information
26102020
HE23-0004
CE 2163

Star Care
NR
No reutilizable
Non-reusable
10 UDS
10 PCS
FFP2
Mascarilla filtrante - NR
Filtering half mask
Ajuste perfecto
Perfect fit
Incluye salvaorejas
Ear saver included
Bolsa zip porta mascarillas
Zip bag for masks
Información técnica
Technical information
26102020
HE23-0004
Star Care
NR
1 UD / 1 PC
FFP2
Mascarilla filtrante - NR
Filtering half mask
Ajuste perfecto
Perfect fit
Incluye salvaorejas
Ear saver included
Bolsa zip porta mascarillas
Zip bag for masks
Información técnica
Technical information
22092020
HE23-0001
CE 2163

3 Straturi

Filtre	Descriere
Filtrul 1	Nețesut: 50 g/m^2
Filtrul 2	Nețesut: 25 g/m^2
Filtrul 3	Topit-suflat (Melt-blown) ≈ 30 g/m2
Filtrul 4	Topit-suflat (Melt-blown) ≈ 30 g/m2
Filtrul 5	Nețesut: 25 g/m^2

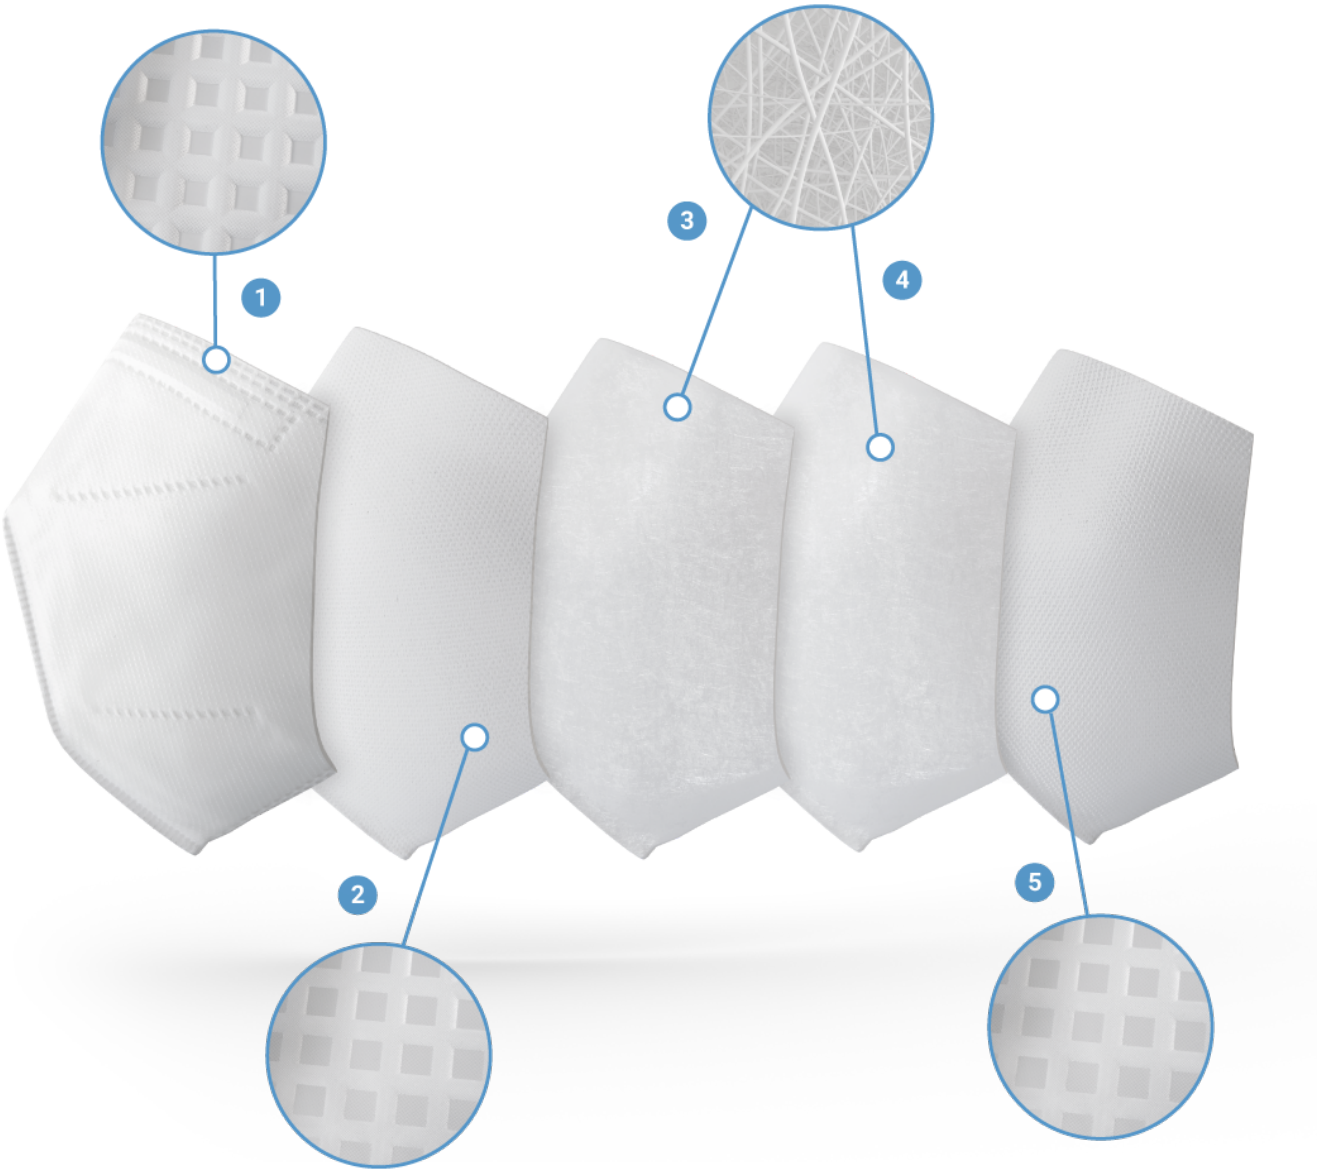

4 PFE

UNE-EN 149:2001	Star Care FFP2 NR mod. MSH	
Eficiența de filtrare necesară a materialului de filtrare pentru aerosoli de NaCl	Certificat nr.: 2163-PPE-707 Certificat nr.: 2163-PPE-707/01	SECRETARIATUL DE STAT PENTRU MUNCĂ ȘI ECONOMIE SOCIALĂ INSTITUTUL NAȚIONAL PENTRU SECURITATE ȘI SĂNĂTATE ÎN MUNCĂ, O.A. M.P CENTRUL NAȚIONAL PENTRU MIJLOACE DE PROTECȚIE * Raport de verificare Centrul Național pentru Mijloace de Protecție (a se vedea anexa 7)
> 94 %	**> 97,35 %**	**> 99 %**

Centru Național pentru Mijloace de Protecție. Centrul Național pentru Mijloace de Protecție (CNMP) face parte din Institutul Național pentru Sănătate și Securitate în Muncă (INSST), un organism științific și tehnic specializat al Administrației Generale de Stat (Spania) a cărui misiune este de a analiza și a studia condițiile de securitate și sănătate la locul de muncă, precum și promovarea acestora și contribuția la îmbunătățirea acestora.

5 Respirabilitate

Materialele selectate oferă o rezistență scăzută la respirabilitate, după cum se poate vedea în grafic, unde toate loturile sunt mult sub limita stabilită de reglementările europene.

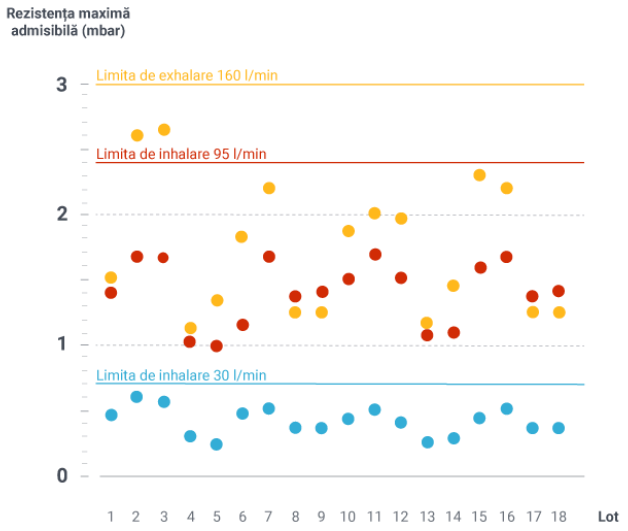

6 Caracteristici suplimentare

1. **Clemă pentru nas ascunsă, conturată**, pentru o mai mare elasticitate
2. **Dimensiuni reglabile** pentru o potrivire perfectă
3. **Benzi elastice plate de 4 mm** pentru o mai bună elasticitate și confort
4. **Sudură dublă** la prinderea benzilor elastice.
5. Îmbinări punctate pentru o filtrare mai eficientă
6. **Protecții pentru urechi pentru confort maxim la utilizarea pe termen lung**
7. **Potrivită pentru uz sanitar.** Încercări suplimentare conform standardului EN 14683 (a se vedea anexa 3)

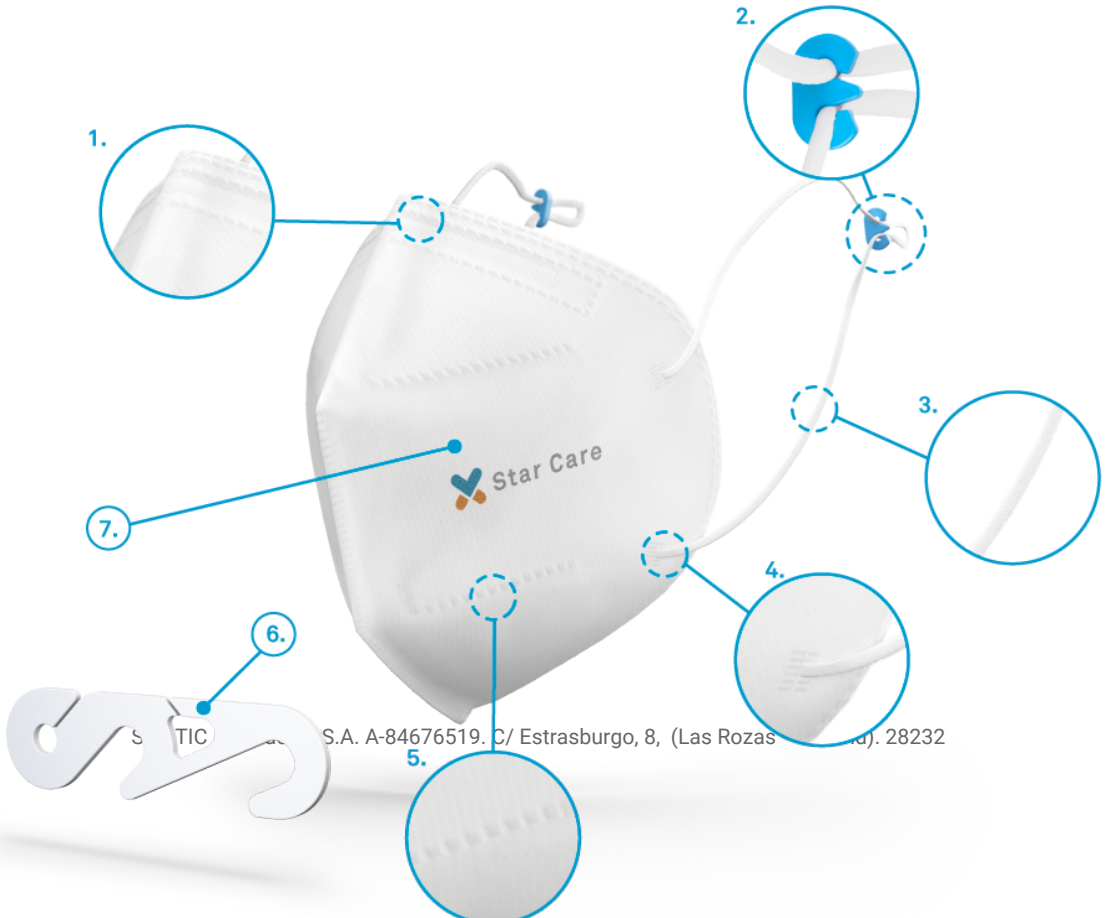

7 Timp de utilizare și depozitare

1. **Pungă port mască** reutilizabilă cu închidere cu fermoar
2. **Ventilație** pentru o depozitare adecvată
3. **Identificator** proprietar
4. **Urmăritor de timp (time tracker)** pentru un control corect al orelor maxime de utilizare

8 Sustenabilitate

1. **Certificare FSC** pentru cutii de cadou din carton (giftbox) din surse durabile (a se vedea anexa 4)
2. **Certificare Soy Ink™** pentru Giftbox (vopseluri vegetale) (a se vedea anexa 5)
3. **Pungă reutilizabilă** compostabilă cu închidere cu fermoar (a se vedea anexa 6)

9 Sistem anti-contrafacere

Autocolant *Produs Original* cu QR care permite accesul la datele specifice ale Controlului de calitate efectuat pe mască și care certifică originalitatea produsului. Include un sigiliu holografic care garantează, de asemenea, inviolabilitatea cutiei.

10 Instrucțiuni de fixare a măștii

1. Țineți masca cu o mână, cu clema pentru nas îndreptată spre degete și benzile elastice atârnând în jos.
2. Așezați masca pe față, acoperind complet nasul și gura. Clema pentru nas trebuie să fie fixată peste nas.
3. Țineți masca cu o mână peste bărbie. Trageți banda elastică și plasați-o în spatele urechii sau fixați-o de protecția pentru urechi pentru un confort sporit.
4. Fixați clema pentru nas cu ambele mâini și asigurați-vă că marginile măștii sunt în contact direct cu fața.
5. Faceți o probă de etanșeitate pentru a verifica dacă ați aplicat corect masca. Cuprindeți masca cu ambele mâini și expirați cu forță. Dacă detectați neetanșeități pe margini, repoziționați masca pe față, reajustați clema pentru nas sau reglați tensiunea benzilor elastice de prindere. Repetați acest proces până când masca este așezată etanș.

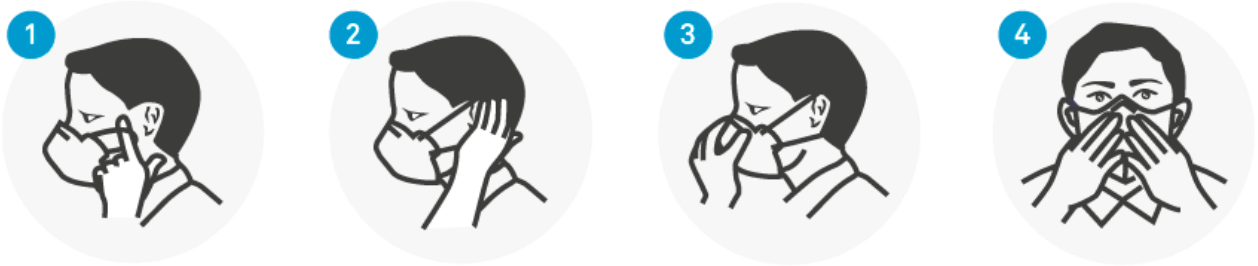

11 Logistica

Pungă individuală

Caracteristici:

Cantitate: 1 unitate/pungă
Dimensiune: 130 x 205 mm
Greutate: 12 g

SKU: MASK-ST-00013.0001

8 436592 290116

Cutie de 10 unități

Caracteristici:

Cantitate: 10 unități (pungi individuale)/cutie
Dimensiune: 131 x 210 x 45 mm
Greutate: 153 g

SKU: MASK-ST-00009.0010

8 436592 290314

Cutie de 50 unități

Caracteristici:

Cantitate: 50 de unități (pungi individuale)/cutie
Dimensiune: 210 x 200 x 131 mm
Greutate: 610 g

SKU: MASK-ST-00013.0050

8 436592 290109

Configurație disponibilă în Q2'2021

Se poate livra în cutie sau într-un alt format în funcție de disponibilitate la momentul comenzii

Master Carton (10)

Caracteristici:

Cantitate: 60 pachete/cutie
Cantitate totală: 600 de unități
Dimensiune: 485 x 415 x 444 mm
Greutate: 10,2 kg

18436592290311

Master Carton (50)

Caracteristici:

Cantitate: 12 pachete/cutie
Cantitate totală: 600 de unități
Dimensiune: 620 x 545 x 234 cm
Greutate: 8,4 kg

18436592290106

Se poate livra în cutie sau într-un alt format în funcție de disponibilitate la momentul comenzii

12 Anexe

12.1 Anexa 1: Declarație de conformitate 14
12.2 Anexa 2: Examinare UE Tip (B) și Certificat de conformitate (C2) 15
12.3 Anexa 3: Raport de încercare EN 14683 (tip IIR) 17
12.4 Anexa 4: Certificat FSC (material carton Giftbox) 22
12.5 Anexa 5: Certificat vopsea vegetală pe bază de soia 23
12.6 Anexa 6: Certificat pungă individuală compostabilă 26
12.7 Anexa 7: Raport de verificare Centrul Național pentru Mijloace de Protecție 28

12.1 Anexa 1: Declarație de conformitate

Prezenta declarație de conformitate, eliberată cu răspunderea exclusivă a producătorului, **Huizhou Hengda Innovation Communication Equipment Co., Ltd.**, situată în Building A, Wanli Industrial Co., Ltd., Dalongkeng, Ganpo, Zhenlong Town, Huiyang District, Huizhou City, Guandgdong Province, China,

CERTIFICĂ

faptul că următorul echipament individual de protecție (PPE)

Model: MSH

Descrierea produsului: Mască de filtrare FFP2

Regulamentul (UE) 2016/425 al Parlamentului European și al Consiliului din 9 martie 2016 privind echipamentele individuale de protecție, inclusiv cerințele esențiale de sănătate și siguranță specificate în anexa II și standardele naționale care transpun următoarele standarde europene armonizate:

EN 149:2001+A1:2009

De asemenea, modelul este identic cu PPE care face obiectul examinării UE de tip [modulul B din Regulamentul (UE) 2016/425] menționat în certificatul nr.:

CE 2163-PPE-707 (Data emiterii: 5.6.2020)

Eliberată de:

Universal Certification and Surveillance Service Trade Ltd. Co. (NB 2163)

Necip Fazil Bulvari Keyap Sitesi E2 Blok NO: 44/84 Yukari Dudullu

Ümraniye-Istanbul

Turcia

Modelul indicat este supus procedurii de evaluare a conformității de tip bazată pe controlul intern al producției plus controlul supravegheat al produselor la intervale aleatorii (modulul C2), în conformitate cu Regulamentul (UE) 2016/425, sub supravegherea organismului notificat Universal Certification and Surveillance Services Trade Co. (NB 2163)

Semnat de către și în numele:

Semnat: Coco Ben

Numele: Coco Ben

Funcția: Director of supply chain

Locul și data: Shenzhen, 05112020

12.2 Anexa 2: Examinare UE Tip (B) și Certificat de conformitate (C2)

UNIVERSAL

UNIVERSAL
CERTIFICATION

NB 2163

EU TYPE EXAMINATION CERTIFICATE

Certificate No: 2163-PPE-707

Respiratory protective devices, filtering half masks to protect against particles manufactured by

Huizhou Hengda Innovation Communication Equipment Co., Ltd.

Building A, Wanli Industrial Co., Ltd., Dalongkeng, Ganpo, Zhenlong Town, Huiyang District, Huizhou City, Guangdong Province, China

are tested and evaluated according to

EN 149:2001 + A1:2009 Respiratory Protective Devices - Filtering Half Masks to Protect Against Particles - Requirements, Testing, Marking

Based on the type examination conducted with the evaluation of test reports, technical file according to Personal Protective Equipment Regulation (EU) 2016/425 Annex 5, it is approved that the product meets the requirements of the regulation.

Product Definition

Brand Name: KSA **Model:** MSH
Filtering half mask
Classification: FFP2 NR

Here by the manufacturer is allowed to use notified body number (2163) and can fix CE mark, as shown below, on the Category III product models given above, with;

- Issuing an appropriate EU Declaration of Conformity according to **Personal Protective Equipment Regulation (EU) 2016/425 Annex 9**.
- Ongoing successful performance in fulfilment of the requirements set out in Personal Protective **Equipment Regulation (EU) 2016/425** and harmonised standards, ensured by assessments based on **Annex 7 (Module C2) or Annex 8 (Module D)** of the regulation no later than 1 year from the beginning of serial production

This certificate is initially issued on **04/06/2020** and will be valid for 5 years, if there is no change in the relevant harmonised standard affecting the essential health and safety requirements.

CE
2163

Suat KAÇMAZ
UNIVERSAL CERTIFICATION
Director

Verify the validity with the QR code

Necip Fazıl Bulvarı Keyap Sitesi E2 Blok No:44/84 Yukarı Dudullu Ümraniye - İSTANBUL - TURKEY T:+90 216 455 80 80
UNIVERSALCERT.COM

UNIVERSAL

UNIVERSAL
CERTIFICATION

NB 2163

EU TYPE EXAMINATION CERTIFICATE

Certificate No: 2163-PPE-707

Respiratory protective devices, filtering half masks to protect against particles manufactured by

Huizhou Hengda Innovation Communication Equipment Co., Ltd.

Building A, Wanli Industrial Co., Ltd., Dalongkeng, Ganpo, Zhenlong Town, Huiyang District, Huizhou City, Guangdong Province, China

are tested and evaluated according to

EN 149:2001 + A1:2009 Respiratory Protective Devices - Filtering Half Masks to Protect Against Particles - Requirements, Testing, Marking

Based on the type examination conducted with the evaluation of test reports, technical file according to Personal Protective Equipment Regulation (EU) 2016/425 Annex 5, it is approved that the product meets the requirements of the regulation.

Product Definition

Brand Name: KSA **Model:** MSH
Filtering half mask
Classification: FFP2 NR

Here by the manufacturer is allowed to use notified body number (2163) and can fix CE mark, as shown below, on the Category III product models given above, with;

- Issuing an appropriate EU Declaration of Conformity according to **Personal Protective Equipment Regulation (EU) 2016/425 Annex 9**.
- Ongoing successful performance in fulfilment of the requirements set out in Personal Protective **Equipment Regulation (EU) 2016/425** and harmonised standards, ensured by assessments based on **Annex 7 (Module C2) or Annex 8 (Module D)** of the regulation no later than 1 year from the beginning of serial production

This certificate is initially issued on **04/06/2020** and will be valid for 5 years, if there is no change in the relevant harmonised standard affecting the essential health and safety requirements.

CE
2163

Suat KAÇMAZ
UNIVERSAL CERTIFICATION
Director

Verify the validity with the QR code

Necip Fazıl Bulvarı Keyap Sitesi E2 Blok No:44/84 Yukarı Dudullu Ümraniye - İSTANBUL - TURKEY T:+90 216 455 80 80
UNIVERSALCERT.COM

12.3 Anexa 3: Raport de încercare EN 14683 (tip IIR)

intertek
Total Quality. Assured.

TEST REPORT NUMBER: PRTT00077512 Page 1 of 6

APPLICANT: STARTIC INNOVACION, S.A. **DATE OF EMISSION:** 16/09/2020

CALLE CASTILLA, No. 18

MADRID, SPAIN
28039

SAMPLE DESCRIPTION:
Type Mask : Medical Face / Type IIR
Reference : Star Care FFP2 NR Mod. MSH
Supplier : Startic Innovacion, S.A.
1 - Medical Face

DATE OF RECEPTION: 01/09/2020

TEST PERFORMED BETWEEN DATES: 01/09/2020 and 16/09/2020

WORK DAYS: 12

REQUEST: Tests performed in accordance with APPLICANT TEST REQUIREMENTS specification

NOTES:

Test	Samples 1
*‡ BFE (FILTRATION)	M
*‡ DIFFERENCIAL PRESSURE (BREATHABILITY)	M
*‡ MICROBIAL CLEANLINESS/BIOBURDEN	M
*‡ SPLASH RESISTANCE PRESSURE	M

M = Meet buyer's requirement; NM = does not meet buyer's requirement; NR = Not requested; NA = Not applicable; NC = No comment; SC = Still continues
- Test results relate only to submitted items. The report shall not be reproduced except in full, without the written approval of Intertek Portugal.
- Tests marked by (*) are not included in the scope of IPAC accreditation for this Laboratory.
- Tests marked by (‡) have been sub-contracted by Intertek Portugal to an accredited laboratory.
- Tests marked by (*‡) are not included in the scope of IPAC Accreditation and have been sub-contracted by Intertek Portugal.
Consult our terms and conditions on http://www.intertek.pt/termos-e-condicoes/.

Textiles Laboratory Manager
ana.morgado@intertek.com

intertek
Total Quality. Assured.

TEST REPORT NUMBER: PRTT00077512 Page 2 of 6

Test Method	Results	Requirements
***‡ BFE (FILTRATION)**		
EN 14683:2019+AC 2019		
	Sample: 1	Type IIR >/= 98%

RESULT

98.1%

Test Conditions:

Temperature: 21±5ºC Humidity: 85±5%

Dimensions of the test specimens: 49cm2 (5 test specimens)

Side of the test specimen facing the challenge aerossol: intern

Air flow rate: 28.3 l/min.

MPS 2.9

Test specimen 1 (98.2%), Test specimen 2 (98.3%), Test specimen 3 (97.7%), Test specimen 4 (98.3%), Test specimen 5 (98.0%).

The expanded uncertainty at a confidence level of 95%, k=2: 1.8%

***‡ DIFFERENCIAL PRESSURE (BREATHABILITY)**

EN 14683:2019+AC 2019

Sample: 1 — Type IIR <60 Pa/cm2

RESULT

47.3 Pa/cm2

Test Conditions:

Temperature: 21±5ºC Humidity: 85±5%

Number and general location of the areas of the mask the differential measurements were taken: Test performed with the direction of flow from the inside to the outside. Side and central location.

Air flow rate: 8L/min

Dimensions of the test specimens: 4.9cm2 (5 test specimens)

Test specimen 1 (46.9 Pa/cm2), Test specimen 2 (48.0 Pa/cm2), Test specimen 3 (46.9 Pa/cm2), Test specimen 4 (46.9 Pa/cm2), Test specimen 5 (48.0 Pa/cm2)

The expanded uncertainty at a confidence level of 95%, k=2: 8.7%

intertek
Total Quality. Assured.

TEST REPORT NUMBER: PRTT00077512

Page 4 of 6

Sample: 1

Type IIR >/= 16.0 kPa

RESULT

Medium pressure test for 29 out of 32 samples as minimum, corresponding to AQL 4%, acording EN 14683: 2019 mask Type IIR)

Sample	Medium Pressure 16.0 Kpa
Amost1	Pass
Amost2	Pass
Amost3	Pass
Amost4	Pass
Amost5	Pass
Amost6	Pass
Amost7	Pass
Amost8	Pass
Amost9	Pass
Amost10	Pass
Amost11	Pass
Amost12	Pass
Amost13	Pass
Amost14	Pass
Amost15	Pass
Amost16	Pass
Amost17	Pass
Amost18	Pass
Amost19	Pass
Amost20	Pass
Amost21	Pass
Amost22	Pass
Amost23	Pass
Amost24	Pass
Amost25	Pass
Amost26	Pass
Amost27	Pass
Amost28	Pass
Amost29	Pass

INTERTEK PORTUGAL UNIPESSOAL, LDA.
Rua Antero de Quental, 221- sala 102, 4455-586 Perafita - Matosinhos
Tel. (+351) 22 999 80 80 - Fax (+351) 22 999 80 81

intertek
Total Quality. Assured.

TEST REPORT NUMBER: PRTT00077512

Page 5 of 6

Sample: 1

Type IIR >/= 16.0 kPa

RESULT

Amost30	Pass
Amost31	Pass
Amost32	Pass

INTERTEK PORTUGAL UNIPESSOAL, LDA.

Rua Ántero de Quental, 221- sala 102, 4455-586 Perafita - Matosinhos
Tel. (+351) 22 999 80 80 - Fax (+351) 22 999 80 81

intertek
Total Quality. Assured.

TEST REPORT NUMBER: PRTT00077512 Page 6 of 6

INTERTEK PORTUGAL UNIPESSOAL, LDA.
Rua Antero de Quental, 221- sala 102, 4455-586 Perafita - Matosinhos
Tel. (+351) 22 999 80 80 - Fax (+351) 22 999 80 81

12.4 Anexa 4: Certificat FSC (material carton Giftbox)

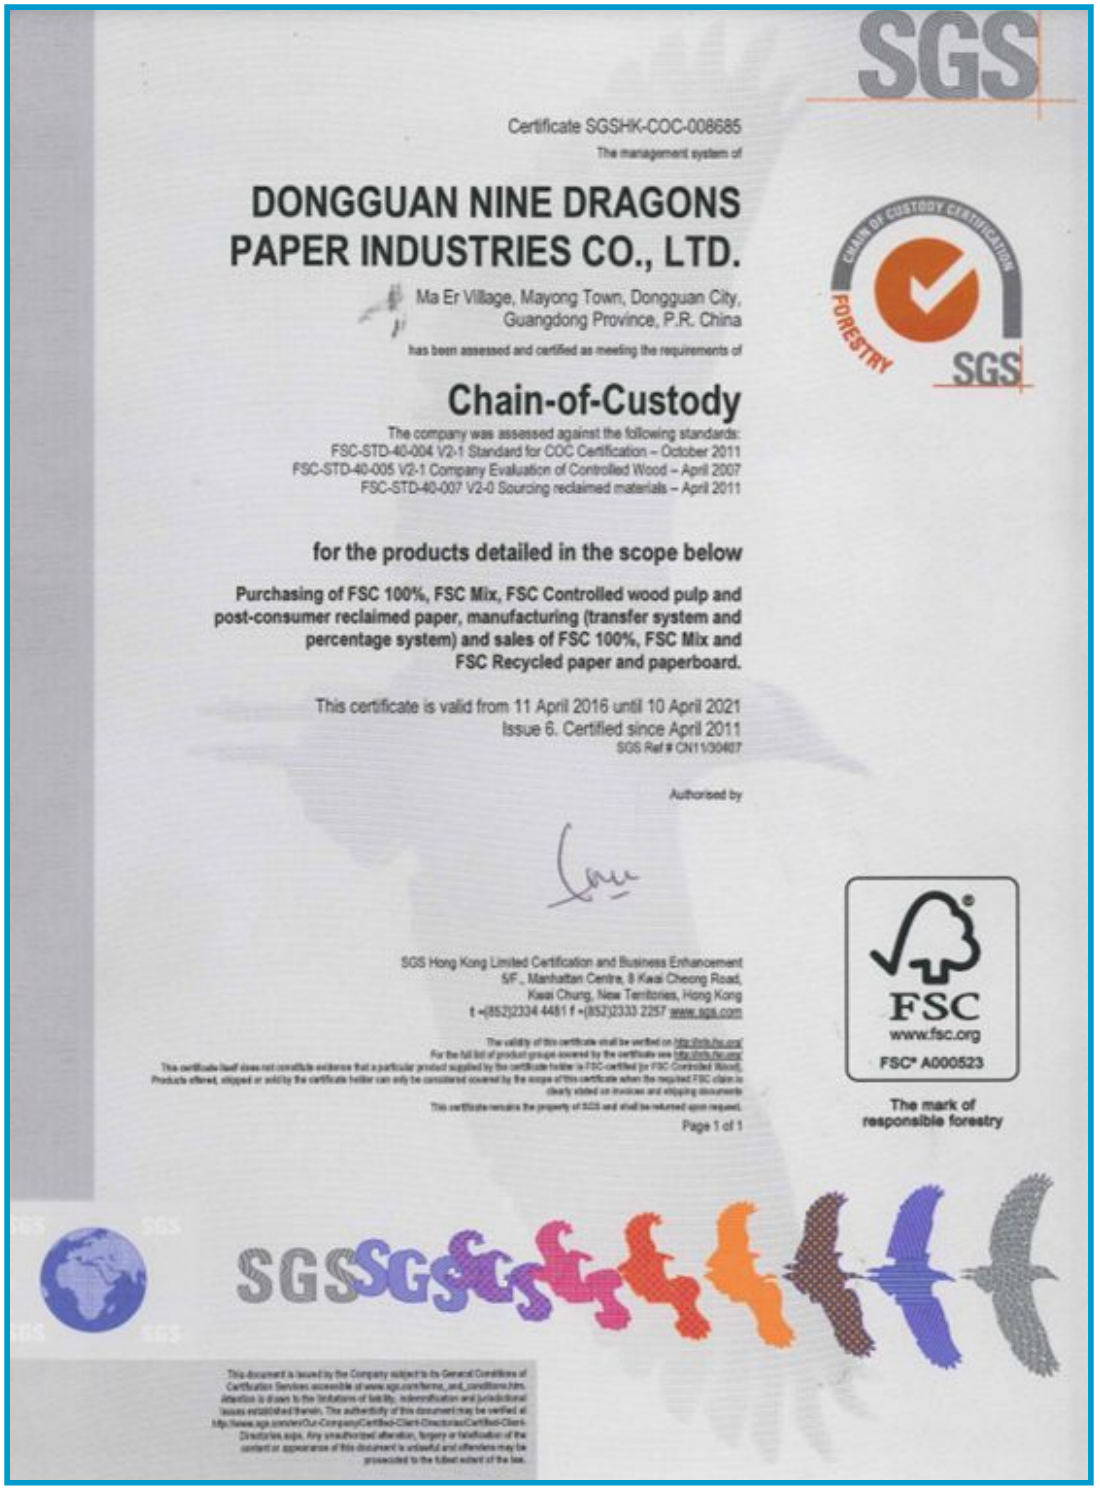

SGS

Certificate SGSHK-COC-008685

The management system of

DONGGUAN NINE DRAGONS PAPER INDUSTRIES CO., LTD.

Ma Er Village, Mayong Town, Dongguan City, Guangdong Province, P.R. China

has been assessed and certified as meeting the requirements of

Chain-of-Custody

The company was assessed against the following standards:
FSC-STD-40-004 V2-1 Standard for COC Certification – October 2011
FSC-STD-40-005 V2-1 Company Evaluation of Controlled Wood – April 2007
FSC-STD-40-007 V2-0 Sourcing reclaimed materials – April 2011

for the products detailed in the scope below

Purchasing of FSC 100%, FSC Mix, FSC Controlled wood pulp and post-consumer reclaimed paper, manufacturing (transfer system and percentage system) and sales of FSC 100%, FSC Mix and FSC Recycled paper and paperboard.

This certificate is valid from 11 April 2016 until 10 April 2021
Issue 6. Certified since April 2011
SGS Ref # CN11/30407

Authorised by

SGS Hong Kong Limited Certification and Business Enhancement
5/F., Manhattan Centre, 8 Kwai Cheong Road,
Kwai Chung, New Territories, Hong Kong
t +(852)2334 4481 f +(852)2333 2257 www.sgs.com

Page 1 of 1

CHAIN OF CUSTODY CERTIFICATION
FORESTRY
SGS

FSC
www.fsc.org
FSC® A000523

The mark of responsible forestry

12.5 Anexa 5: Certificat vopsea vegetală pe bază de soia

ASA
American Soybean Association®

SOYINK LICENSE AGREEMENT

This agreement is made as of this 2nd day of January, 2020, by the **American Soybean Association** ("ASA") and Maoming Sakata Inx Co., Ltd. ("Licensee"), located at 12th sub-district, Nanhai eastern area, Dianbai district, Maoming City, Guangdong, China.

ASA is the owner of the "Printed with Soy Ink" certification mark (the "SoySeal") and has established minimum standards for use of the SoySeal.

Licensee is applying to ASA for the right to use the SoySeal on materials printed with ink containing soybean oil/soy protein.

The parties hereto agree as follows:

I. **MINIMUM STANDARDS.** The SoySeal may be used by Licensee only on products meeting or exceeding the following established standards.

Soybean oil* as a percentage of total formula weight

TYPE OF INK	*% SOY OIL CONTENT
Black news ink	40
Color news ink	30
Cold-set ink	30
Carbon ink	25
Screen printing ink	25
Sheet-fed ink	20
Business forms ink	20
Metallic ink	10
Desensitizing ink	10
Heat-set ink	7
UV/EB ink	7
Stencil duplicator ink	6

*Soybean oil must be the predominant vegetable oil, with vegetable drying oils added as needed, but not to exceed the level of soybean oil set out in the respective formulation. Alcohol esters of soybean oil may be substituted directly for soybean oil in news, sheet-fed, cold-set and business forms inks to obtain the minimum concentration standard. The minimum soybean oil concentration for heat-set inks increased to 15% (by weight) when alcohol esters of soybean oil replace soybean oil in this formulation.

Flexographic ink: This vehicle must contain a minimum of 20% soy protein; (water based) a minimum of 15% of the vehicle must be included in the ink.

II. **GRANT.** ASA hereby grants to Licensee a non-exclusive right to use the SoySeal on Licensees' publications, labels, packages and other promotional and merchandising material, subject to the requirements of this Agreement. If the Licensee has more than one office or satellite location, each location will be required to have its own agreement.

III. **ROYALTIES.** For and in consideration of the mutual promises herein, the Licensee shall pay ASA the sum of Three Hundred Fifty Dollars ($350) per year, payable on or before January 1.

The royalty will be adjusted based on the quarter in which the agreement is executed.

January – March	April – June	July – September	October - December
100% or $350	75% or $262.50	50% or $175	25% - $87.50

IV. **DESCRIPTION AND USE.** ASA shall provide artwork of the SoySeal mark upon payment of the annual royalty. The SoySeal mark is to be clearly and distinctly affixed to product labels and packages to provide ready recognition that the ink contains soybean oil/soybean protein. The Licensee agrees to use the SoySeal mark in accordance with the standards for use of the SoySeal, as established in Item I.

The Licensee herein agrees that it shall use the trademark registered notice where the SoySeal mark is most prominently displayed upon a label, the product, in advertising, and the like, by applying the symbol '®' to the mark where it is most prominently displayed.

V. **TERMINATION OF CONTRACT.** Licensee is to cease using the SoySeal upon written notice by ASA to Licensee in the event, in ASA's sole judgment based on analytical findings, the ink does not meet the minimum standards as defined on Page 1 of this Agreement, or is not complying with the other terms and conditions of this agreement.

VI. **INDEMNIFICATION.** Licensee shall indemnify and hold harmless ASA's officers, directors, agents and assigns from and against all claims, actions, damages, expenses (including, but without limitation, reasonable attorney's fees) and liability whatsoever, arising out of or in conjunction with any breach of this Agreement by Licensee.

VII. **ASSIGNMENT/SUBLICENSING RESTRICTION.** The right to use the SoySeal herein may not be assigned or sublicensed without prior written consent of ASA.

VIII. **COMPLIANCE/AUTHORIZATION.** A sample of the packaging and a description of the ink (by brand name and type of formulation) that is to be certified must be supplied if requested by ASA.

Licensee also agrees to provide a description of all products/printed materials on which the SoySeal is being applied. Licensee is authorized to use the SoySeal on the following:

Product/Publication C Ecopure/Sheet-fed ink

Product/Publication Web C Master/Cold-set ink Web C Master/Heat-set ink

Product/Publication Dreamcure/UV ink

Please attach a separate sheet for any additional product/publication descriptions.

AMERICAN SOYBEAN ASSOCIATION

Signature

2/3/20
Date

AMERICAN SOYBEAN ASSOCIATION

LICENSEE

YUANYUN ZHOU
Name – Please Print

YUANYUN ZHOU
Signature

Quality Assurance Director
Title

(0086) 0668-2089301
Phone Number

(0086) 0668-2689966
Fax Number

zhouyuanyun@inx-sm.com
Email

January. 02. 2020
Date

Please forward the signed user agreement to:

Farris Haley
American Soybean Association
12125 Woodcrest Executive Drive, Suite 100
St. Louis, MO 63141
Phone : 1.800.688.7692
Fax: 314.754.1284 or 314.576.2786
Email: fhaley@soy.org

V. 04/01/09

12.6 Anexa 6: Certificat pungă individuală compostabilă

CERTIFICATE

for Products

THIS IS TO CERTIFY that the following PRODUCTS have been found to comply with the specifications established in the American Society for Testing and Materials standard ASTM D6400 and/or D6868 in accordance with the terms and conditions of the "International Biodegradable Products Institute, Inc. Licensing & Certification Program for Compostable Products":

- Colored Ziplock Bag 1800 Microns [20180807-01]

as further described in the application and related information submitted to the Biodegradable Products Institute by Dongguan Xinhai Environment-Friendly Materials Co., Ltd. Corporation, (the "Licensee") a corporation of China.

Specific products associated with these certifications can be found on the BPI Product Catalog: https://products.bpiworld.org/companies/dongguan-xinhai-environment-friendly-materials-co-ltd

This Certificate authorizes the Licensee to use the Certification Program Logo depicted below in relation to such Product , subject to all conditions and terms of the Program Rules and the License Agreement between the Biodegradable Products Institute and the Licensee.

BPI COMPOSTABLE

COMMERCIALLY COMPOSTABLE ONLY. FACILITIES MAY NOT EXIST IN YOUR AREA.
CERT #7719318

By: _____
BPI Executive Director

Valid until: March 31, 2022
Certificate #: 7719318-5

Products on this Certificate:

The following item numbers (SKUs) are certified under this document. Only these items are published on the BPI's web-based products catalogs.

The licensee shall inform BPI immediately for any new products or discontinued products. These products were certified under product review 20180807-01 and must be recertified by the BPI on or before March 03, 2022

Brand	Manufacturer SKU	Title
XHBIO	XH-ZB	Colored Ziplock Bag

12.7 Anexa 7: Raport de verificare Centrul Național pentru Mijloace de Protecție

MINISTERIO
DE TRABAJO
Y ECONOMIA SOCIAL

SECRETARÍA DE ESTADO DE
EMPLEO Y ECONOMIA SOCIAL

INSTITUTO NACIONAL DE
SEGURIDAD Y SALUD
EN EL TRABAJO, O.A., M.P.

CENTRO NACIONAL DE
MEDIOS DE PROTECCIÓN

21336920

Página 1 de 3

Informe de ensayo, referido a la mascarilla autofiltrante (media máscara filtrante) frente a partículas, Mascarilla FFP2, [redacted]

Este informe, que consta de tres páginas numeradas y selladas, sólo puede ser reproducido en su totalidad. En cualquier otro caso deberá mediar la autorización escrita de la Directora del Centro Nacional de Medios de Protección. La información detallada relativa a los ensayos realizados está a disposición del cliente, previa solicitud por escrito.

1. Antecedentes.

Con fecha 30 de julio de 2020 y con número de registro de entrada (NRE) 03687 se recibió en el Centro Nacional de Medios de Protección (CNMP) solicitud formal de ensayos de la mascarilla autofiltrante (media máscara filtrante) frente a partículas Mascarilla FFP2, [redacted]

2. Objeto.

Describir los resultados de los siguientes ensayos:

- Penetración con aerosol de NaCl (en estado de recepción)

realizados a las muestras recibidas cuya clasificación es FFP2 indicada por el solicitante, conforme a lo establecido en las normas:

UNE-EN 149:2001+A1:2010 "Dispositivos de protección respiratoria. Medias máscaras filtrantes de protección contra partículas. Requisitos, ensayos, marcado".

UNE- EN 13274-7:2008 "Equipos de protección respiratoria. Métodos de ensayo. Parte 7: Determinación de la penetración de los filtros de partículas".

3. Muestras.

3.1. Recepción.

Nº muestras	Fecha entrada CNMP	Códigos de identificación
3	29.07.2020 / 1034	del 36920-01 al 36920-3

3.2. Descripción.

Esta descripción se realiza basándose en una inspección visual (véanse fotografías).

Son mascarillas autofiltrantes o medias máscaras filtrantes, plegadas, sin válvula de exhalación. Disponen de clip nasal. El arnés de cabeza consiste en cintas elásticas que pasan por las orejas.

ENAC
ENSAYOS
Nº 1108/LE2151

Los ensayos marcados (*) no están amparados por la acreditación ENAC.

CORREO ELECTRÓNICO
cnmp@insst.mitramiss.es

CARABELA LA NIÑA, 16
41007 SEVILLA
TEL: 95 451 41 11
FAX: 95 467 27 97
Código DIR3: EA0041505

Centro Nacional de Medios de Protección

Informe 21336920

Las muestras se presentan en bolsa de plástico de 1 ud.

Marcado

En el lateral izquierdo indica Star Care CE 2163 EN 149:2001+A1:2009 FFP2 NR MSH

Fotografías

4. Ensayos.

Los ensayos fueron realizados según lo indicado en la siguiente tabla.

Ensayo (UNE-EN 149:2001+A1:2010)	Procedimiento	Fecha de realización
Penetración con aerosol de NaCl en estado de recepción 8.11 (y UNE-EN 13274-7:2008)	MPE-2221	25-08-20

MINISTERIO DE TRABAJO Y ECONOMÍA SOCIAL C.N.M.P. - SEVILLA Instituto Nacional de Seguridad y Salud en el Trabajo O.A. M.P.

MINISTERIO
DE TRABAJO
Y ECONOMÍA SOCIAL

INSTITUTO NACIONAL
DE SEGURIDAD Y SALUD
EN EL TRABAJO, O.A., M.P.

CENTRO NACIONAL DE
MEDIOS DE PROTECCIÓN

Centro Nacional de Medios de Protección

Informe 21336920

Página 3 de 3

5. Resultados y conformidad.

A continuación se muestran los resultados obtenidos de los ensayos y determinaciones realizados, **que sólo son válidos para las muestras ensayadas.**

Ensayo	Especificación (UNE-EN 149:2001+A1:2010)	Resultado	Conclusión[1]
Penetración del material filtrante frente a aerosol de NaCl en estado de recepción (Penetración después de 3,5 minutos)	7.1, 7.2, 7.9.2 Penetración del material filtrante Clasificación FFP2 ≤ 6 %	(%) 1,025 ± 0,002 0,963 ± 0,002 0,564 ± 0,002	Cumple FFP2

(1) La clasificación final de una mascarilla tipo FFP según UNE-EN 149 viene determinada por los resultados de un conjunto de ensayos y no sólo por el aquí reflejado.

Sevilla, a 03 de septiembre de 2020

Mª Angeles Serra de Torres
Técnico Superior de Prevención
Unidad Técnica Protección Respiratoria

MINISTERIO DE TRABAJO Y ECONOMÍA SOCIAL · C.N.M.P. · SEVILLA · Instituto Nacional de Seguridad, Salud e Higiene O.A. M.P.

MINISTERIO DE TRABAJO Y ECONOMÍA SOCIAL
INSTITUTO NACIONAL DE SEGURIDAD Y SALUD EN EL TRABAJO, O.A., M.P.
CENTRO NACIONAL DE MEDIOS DE PROTECCIÓN